


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
Data File : BF131704.D
Acq On : 20 Dec 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 21 03:12:37 2022

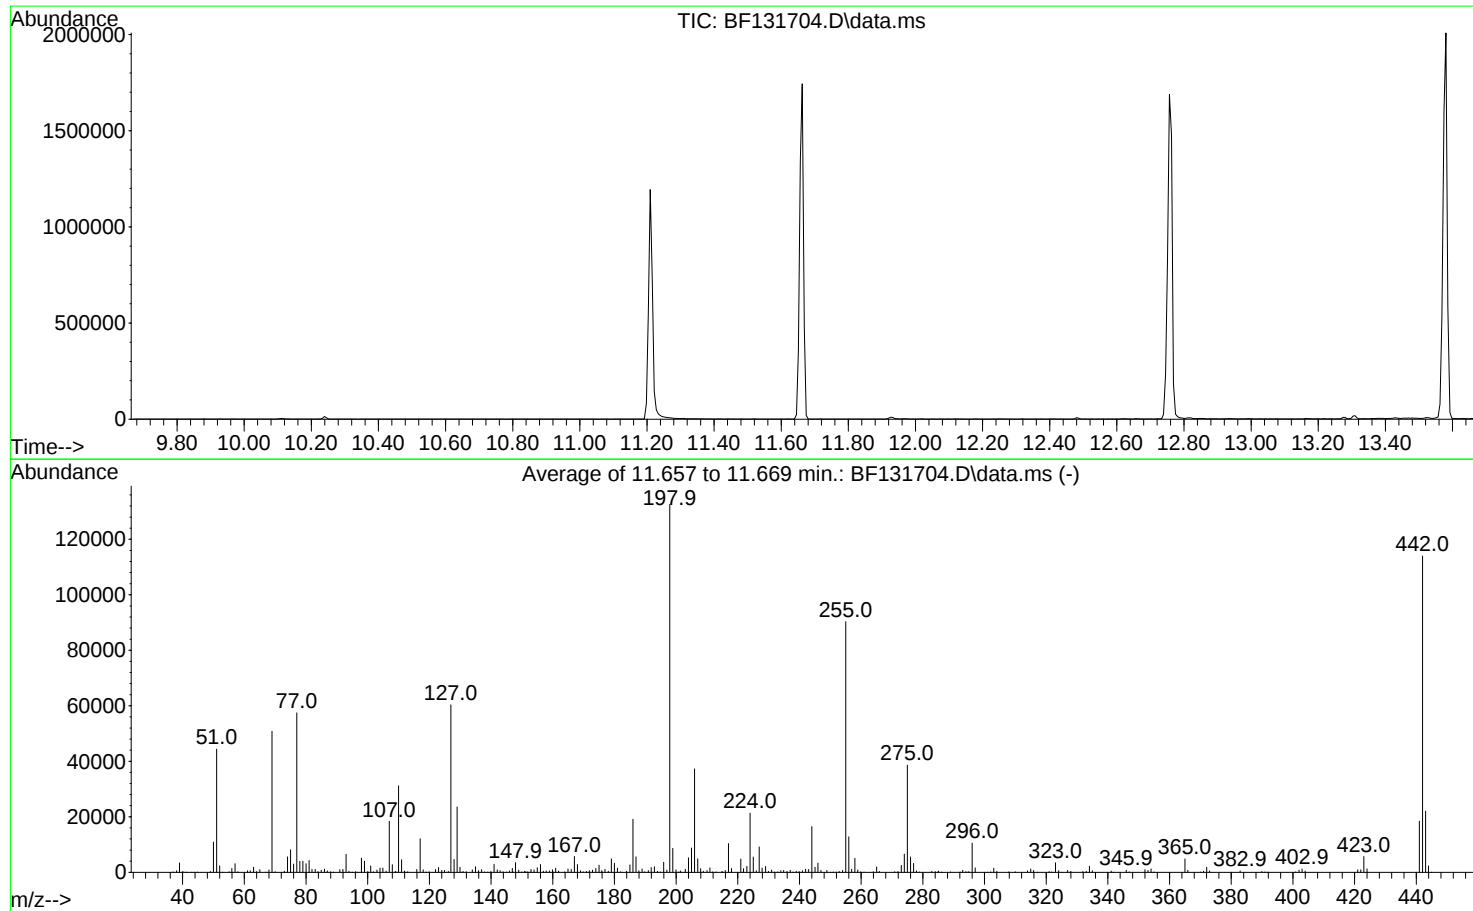




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	44404	PASS
68	69	0.00	2	1.7	870	PASS
69	198	0.00	100	38.4	50841	PASS
70	69	0.00	2	0.5	238	PASS
127	198	10	80	45.5	60348	PASS
197	198	0.00	2	0.6	792	PASS
198	198	100	100	100.0	132565	PASS
199	198	5	9	6.5	8651	PASS
275	198	10	60	29.1	38608	PASS
365	198	1	100	3.7	4840	PASS
441	198	0.01	100	13.9	18426	PASS
442	442	50	100	100.0	113965	PASS
443	442	15	24	19.4	22063	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
Data File : BF131704.D
Acq On : 20 Dec 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 21 06:25:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

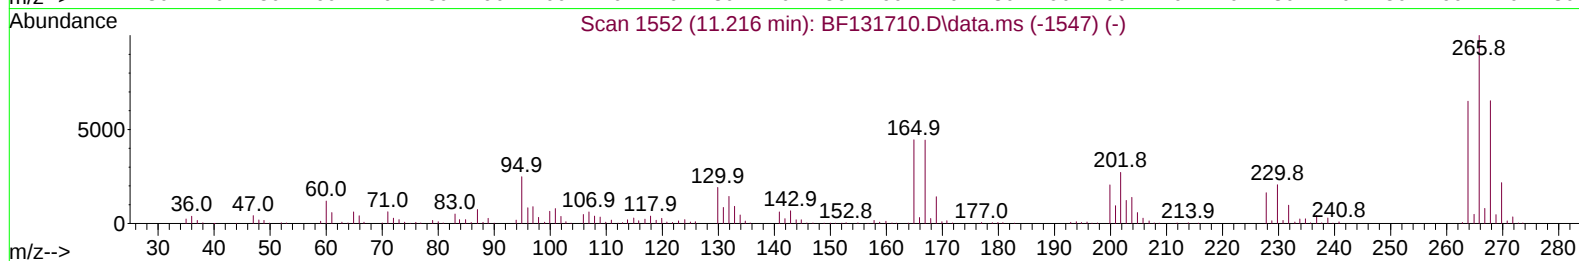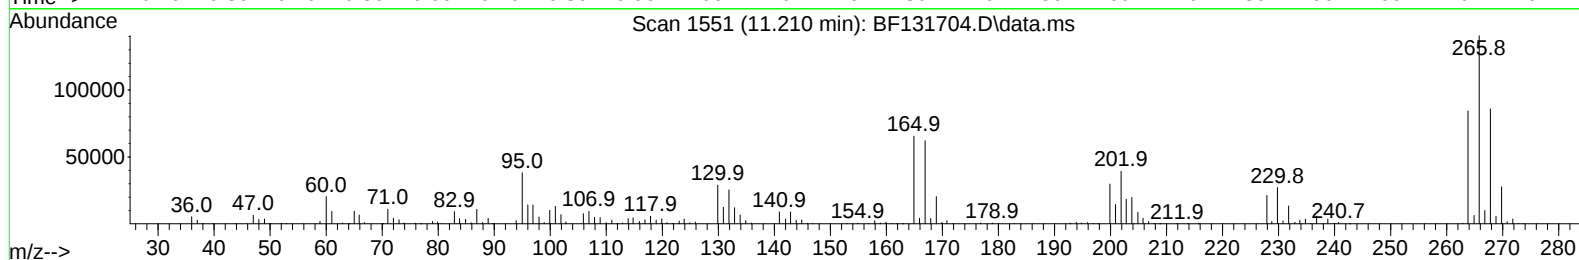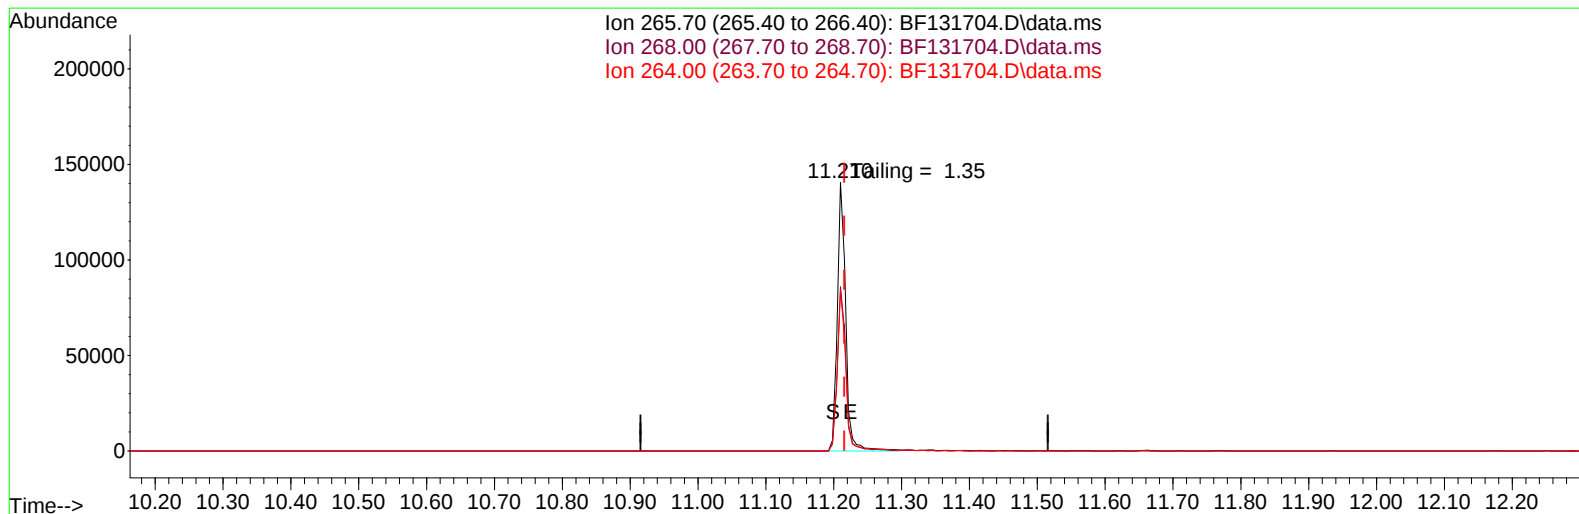

TIC: BF131704.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 25823.55 ng




response 121063

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.17
264.00	65.00	60.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
 Data File : BF131704.D
 Acq On : 20 Dec 2022 10:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 21 06:25:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 03:12:37 2022
 Response via : Initial Calibration

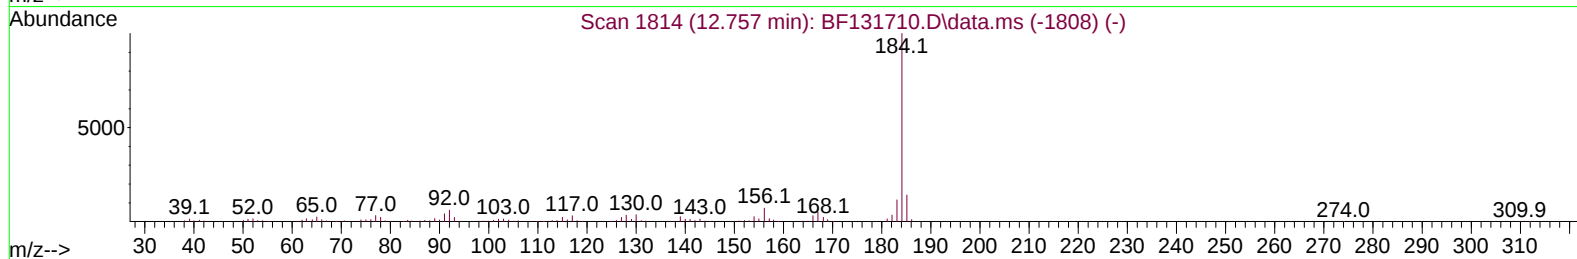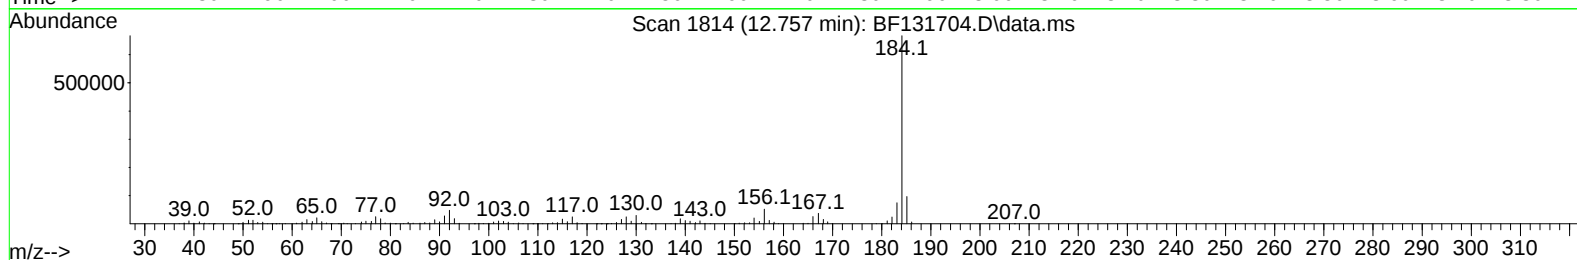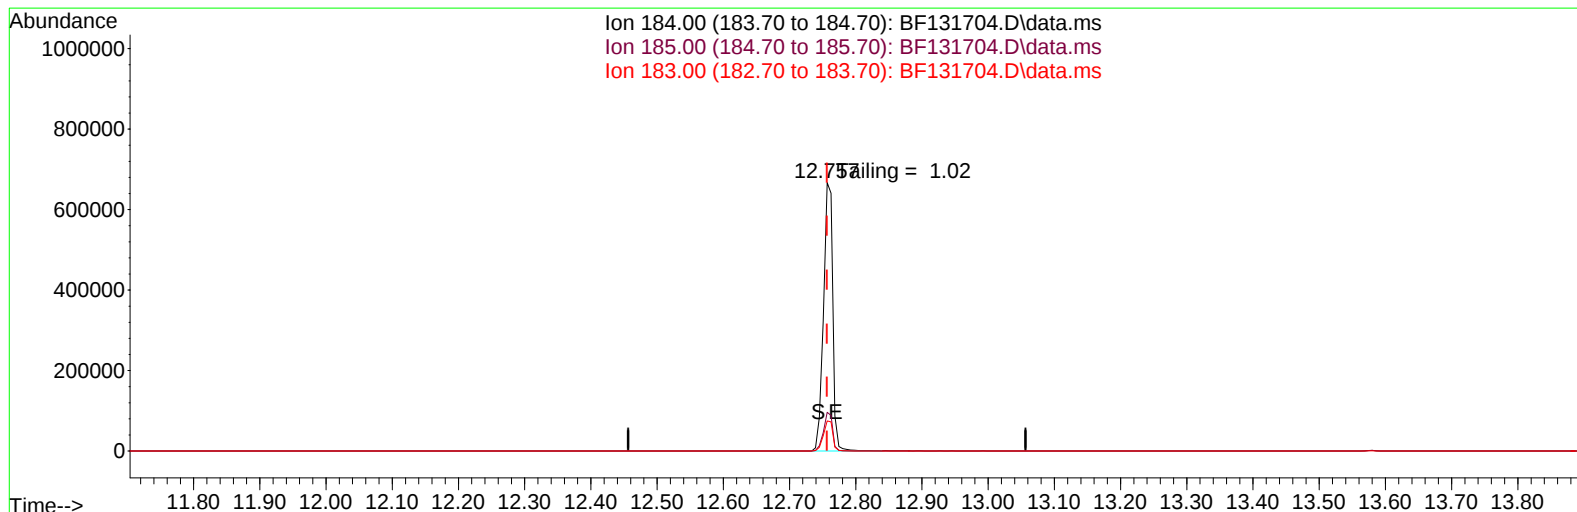

TIC: BF131704.D\data.ms

(77) Benzidine

12.757min (+ 0.000) 0.00 ng

response 652637

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.47
183.00	11.60	11.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2022	BNA_F	<u>BF131704.D</u>
Compound Name	Response	Retention Time
DDT	339530	13.58
DDD	4838	13.31
DDE	358	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5196	344726	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP