


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
 Data File : BF131716.D
 Acq On : 20 Dec 2022 16:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 03:12:37 2022

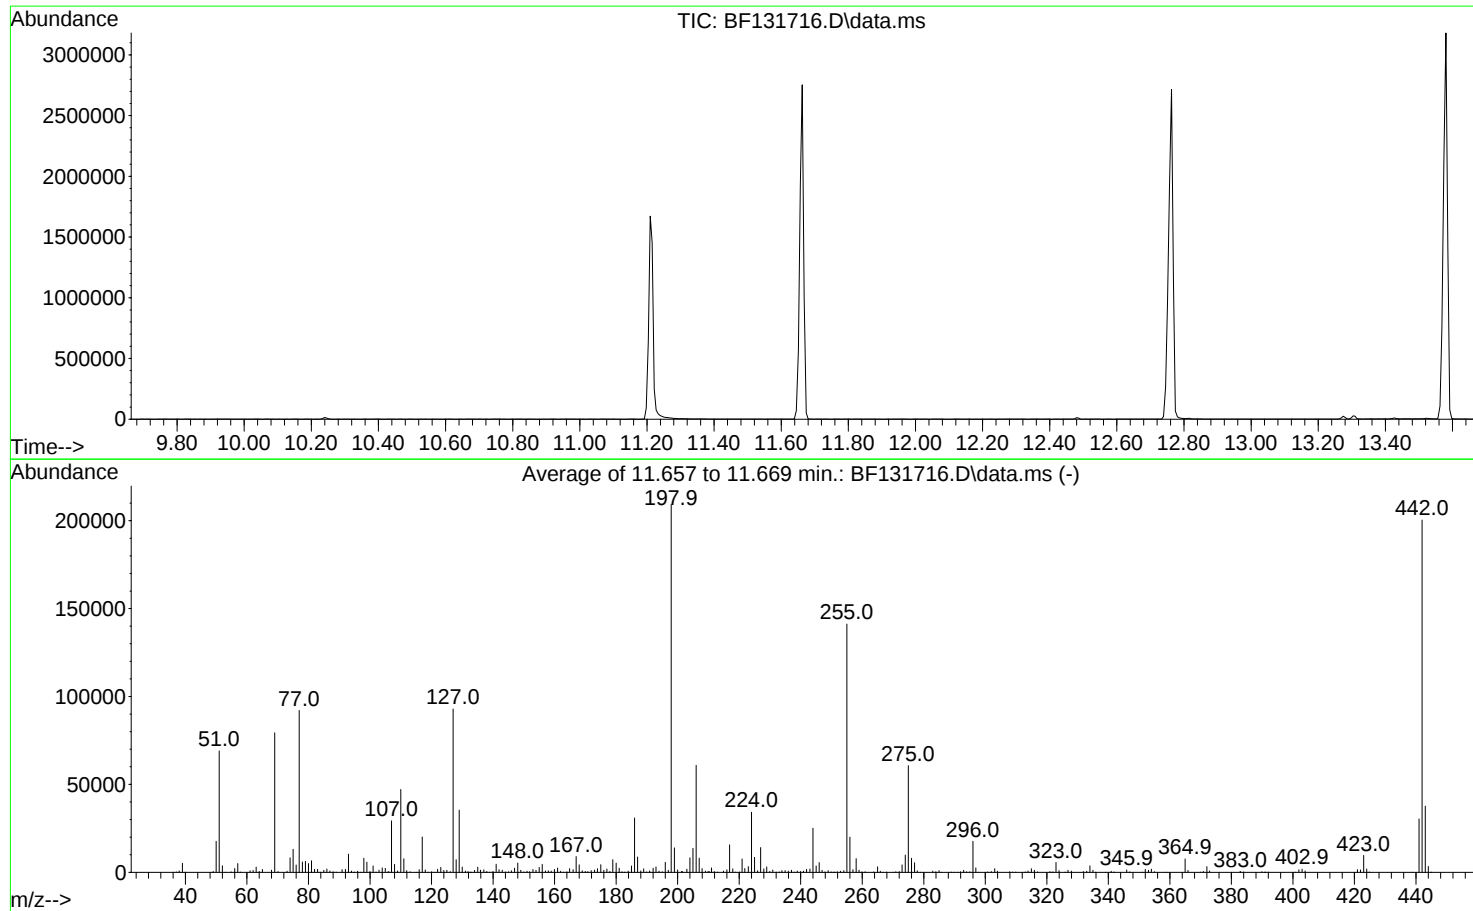




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	69035	PASS
68	69	0.00	2	1.6	1256	PASS
69	198	0.00	100	37.9	79339	PASS
70	69	0.00	2	0.5	389	PASS
127	198	10	80	44.4	92896	PASS
197	198	0.00	2	0.6	1152	PASS
198	198	100	100	100.0	209248	PASS
199	198	5	9	6.7	13915	PASS
275	198	10	60	29.0	60664	PASS
365	198	1	100	3.6	7622	PASS
441	198	0.01	100	14.5	30339	PASS
442	442	50	100	100.0	200395	PASS
443	442	15	24	18.8	37632	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\
Data File : BF131716.D
Acq On : 20 Dec 2022 16:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 21 06:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

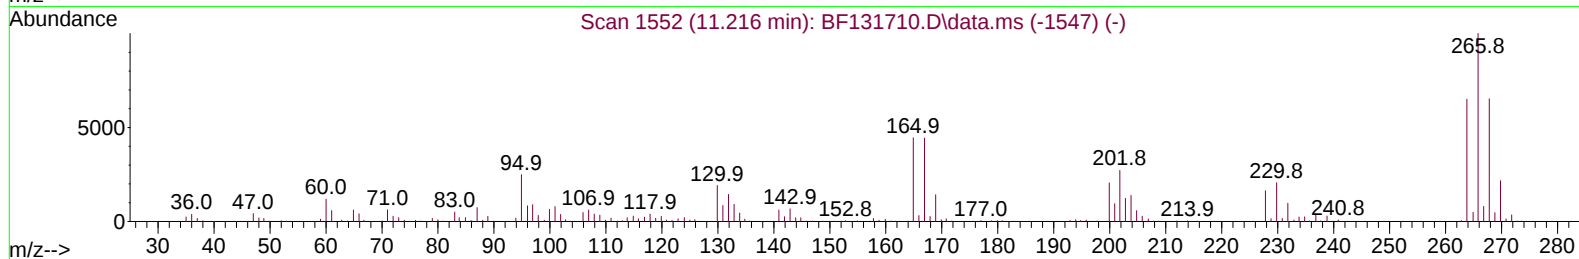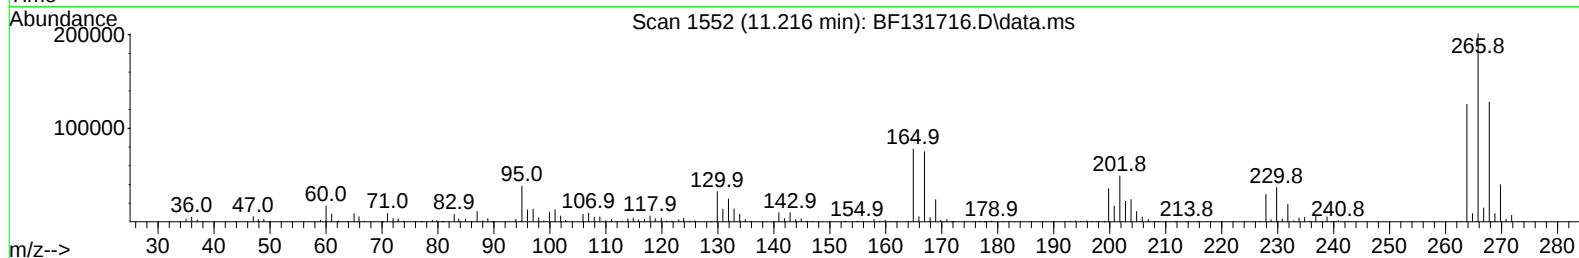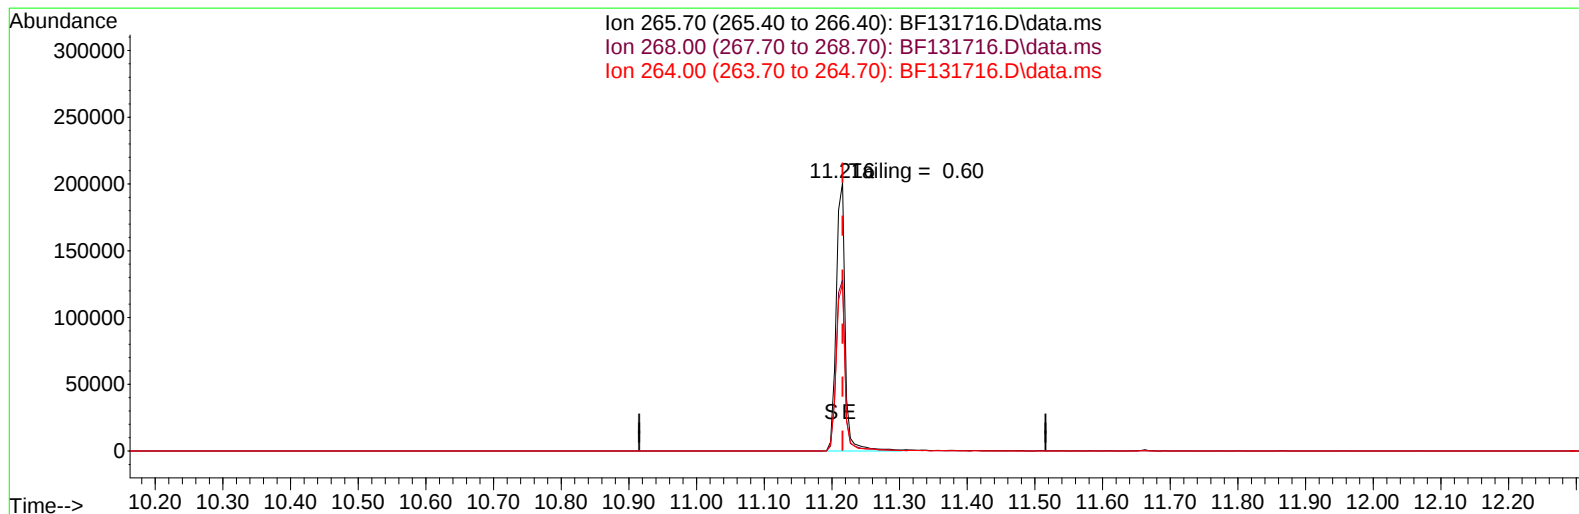

TIC: BF131716.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.000) 488275.70 ng




response 185146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.67
264.00	65.00	62.49
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122022\  
Data File : BF131716.D  
Acq On    : 20 Dec 2022  16:48  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 21 06:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

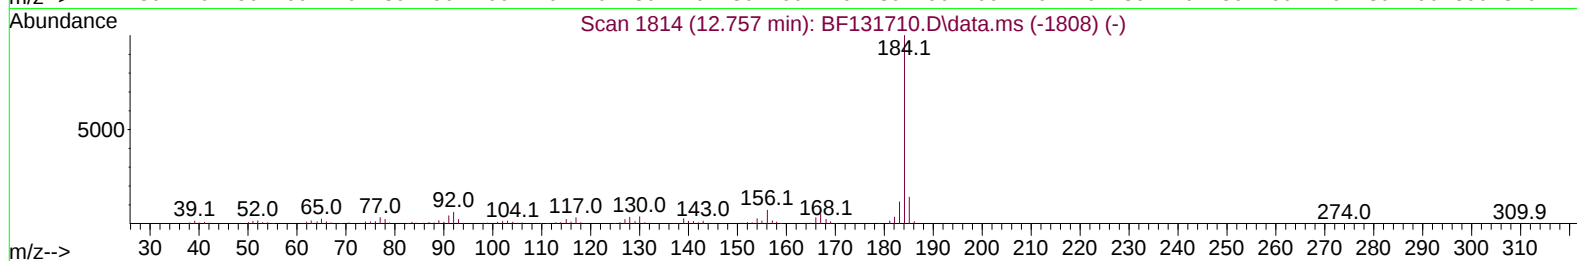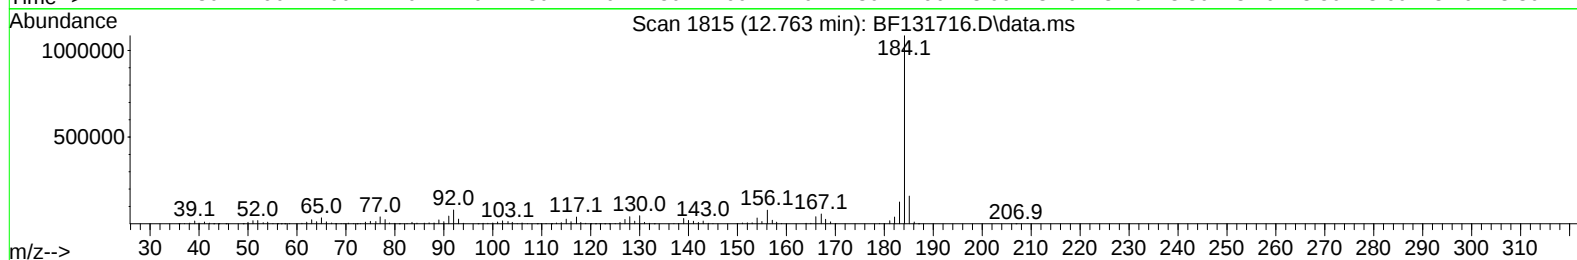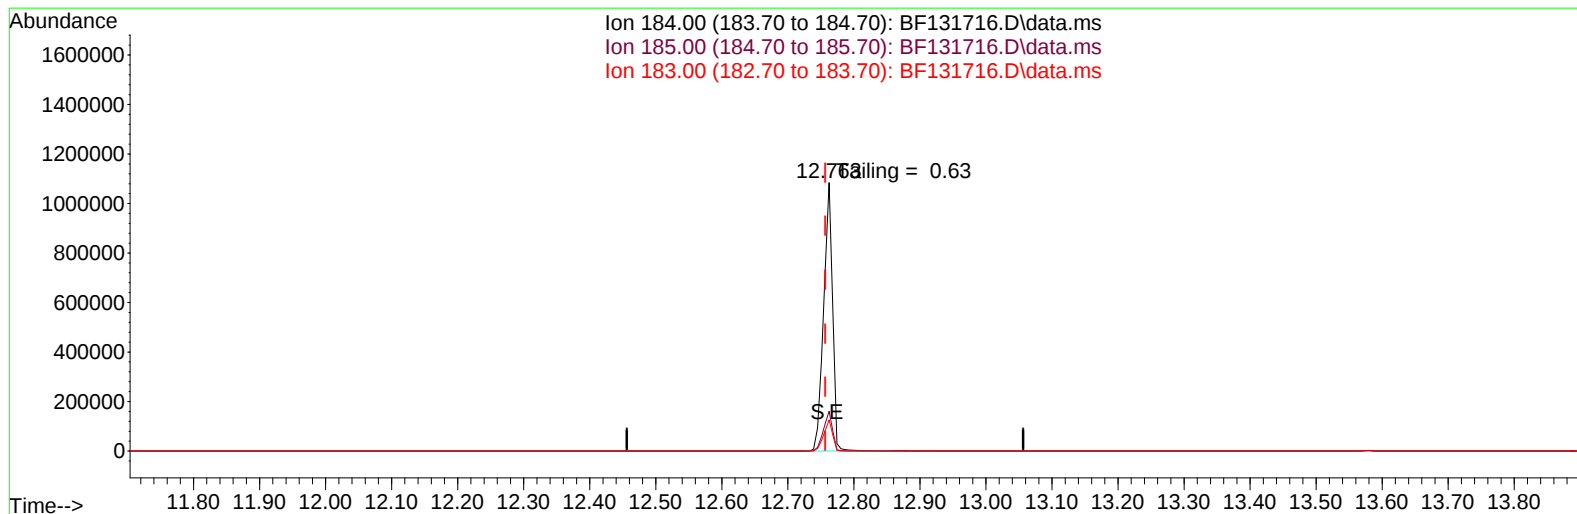

TIC: BF131716.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response **1021042**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.77
183.00	11.60	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2022	BNA_F	<u>BF131716.D</u>
Compound Name	Response	Retention Time
DDT	540680	13.58
DDD	9385	13.31
DDE	63	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9448	550128	1.72

Instrument :
BNA_F
ClientSampleId :
DFTPP