
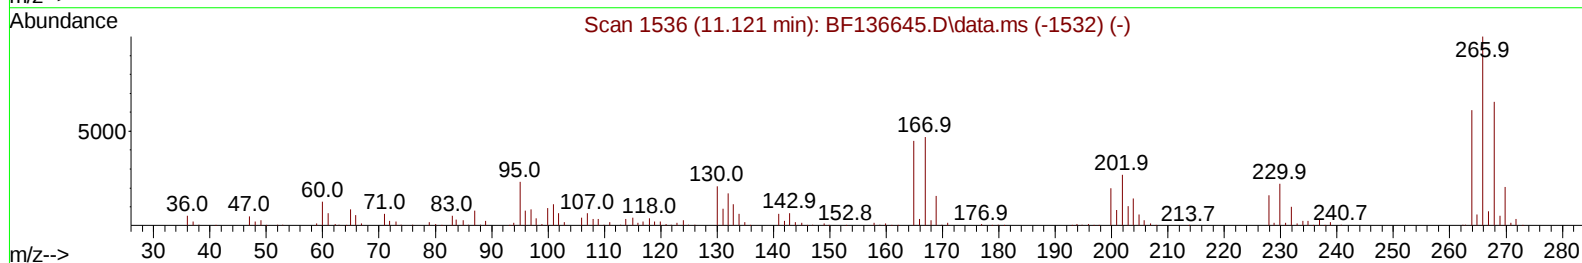
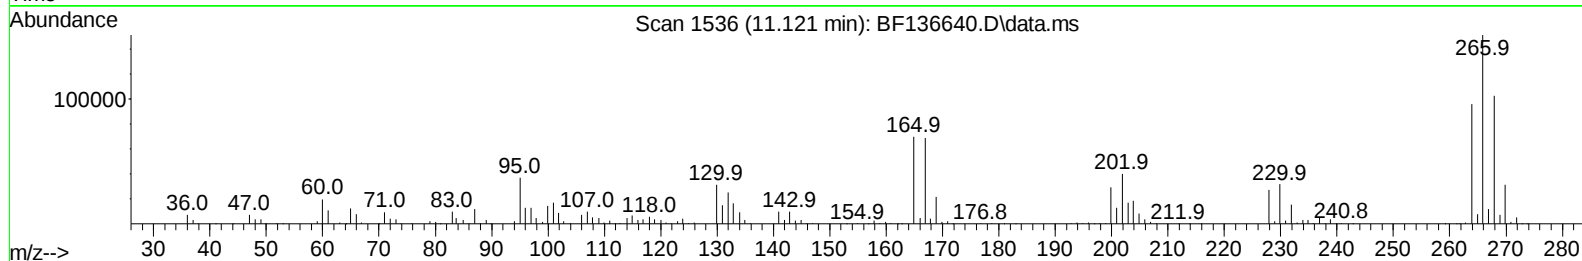


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136640.D
Acq On : 20 Dec 2023 08:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 16:17:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 15:40:36 2023
Response via : Initial Calibration

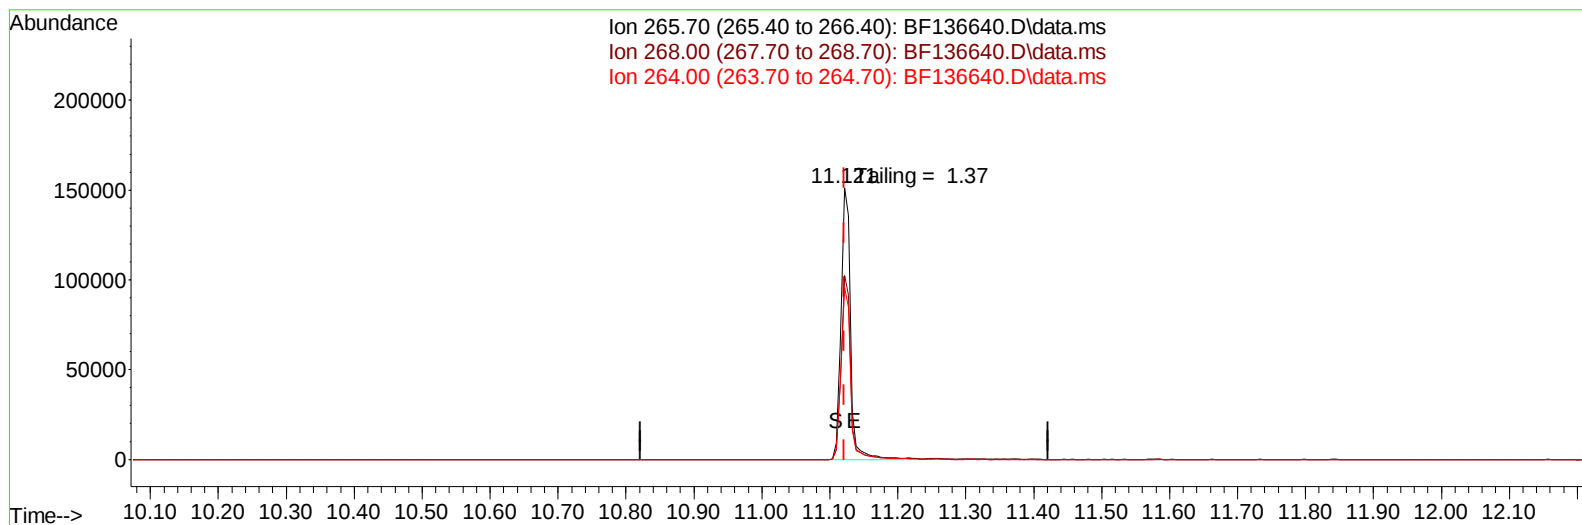




TIC: BF136640.D\data.ms

(70) Pentachlorophenol (C)**11.121min (-0.000) 35779.06 ng****response 146132**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.69
264.00	61.20	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136640.D
Acq On : 20 Dec 2023 08:45
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 16:17:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 15:40:36 2023
Response via : Initial Calibration

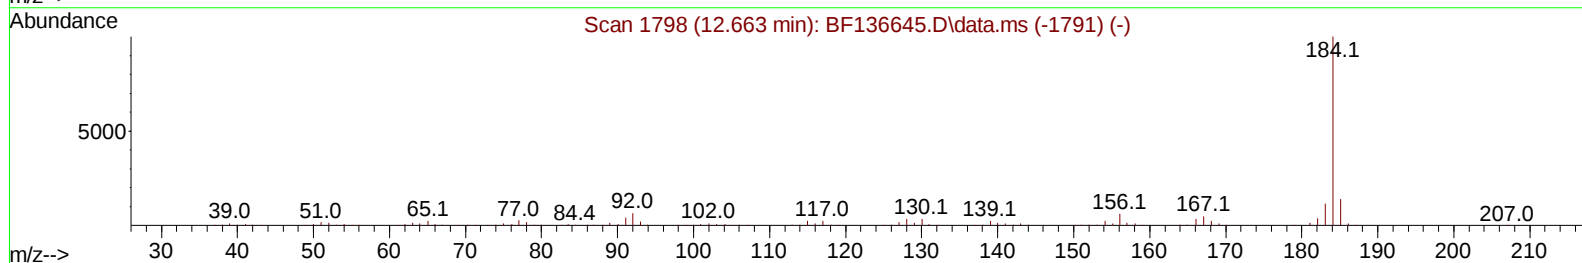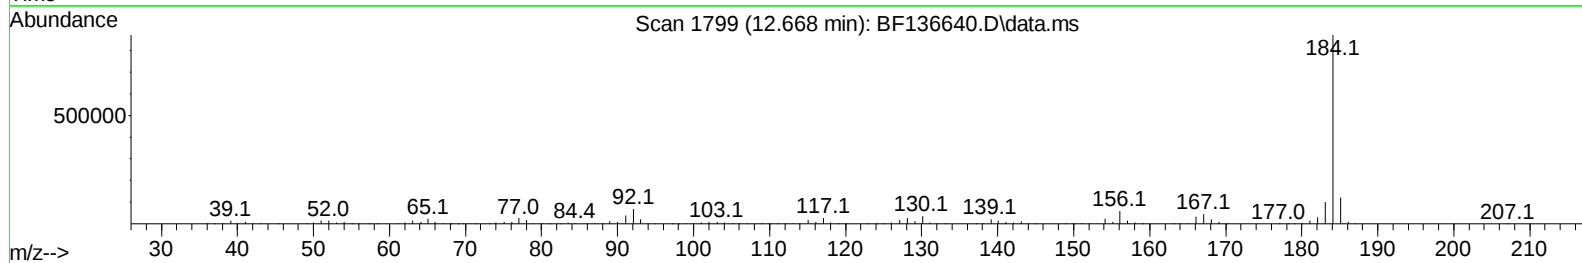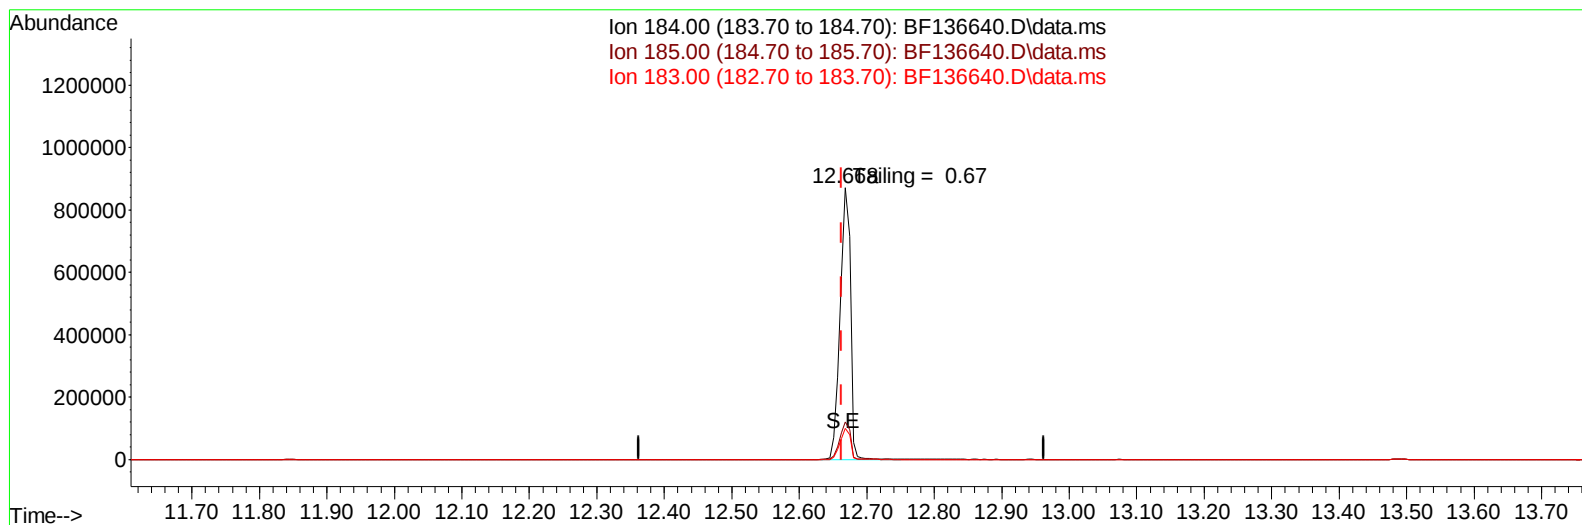

TIC: BF136640.D\data.ms

(77) Benzidine**12.668min (+ 0.006) 0.00 ng****response 918090**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.85
183.00	11.60	11.54
0.00	0.00	0.00