

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
 Data File : BF136655.D
 Acq On : 20 Dec 2023 19:05
 Operator : CG\JU
 Sample : PB157610BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157610BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	8	14	rVB	29301	41787	1.37%	0.242%
2	5.446	565	571	574	rBV	2136208	2251750	73.91%	13.063%
3	6.440	734	740	743	rBV	2074649	2294436	75.32%	13.311%
4	6.793	796	800	803	rBV	482484	431192	14.15%	2.502%
5	7.351	889	895	898	rBV	1296244	1484125	48.72%	8.610%
6	8.063	1012	1016	1020	rBV	630832	585925	19.23%	3.399%
7	9.145	1194	1200	1203	rBV	2961701	2860634	93.90%	16.596%
8	9.822	1310	1315	1318	rBV	831919	694304	22.79%	4.028%
9	10.616	1445	1450	1453	rBV	1765045	1693931	55.60%	9.827%
10	11.316	1565	1569	1572	rBV	859595	777508	25.52%	4.511%
11	12.916	1835	1841	1844	rBV	3051205	3046409	100.00%	17.673%
12	13.963	2015	2019	2023	rBV	610168	531811	17.46%	3.085%
13	15.439	2265	2270	2275	rBV	302211	399756	13.12%	2.319%
14	15.486	2275	2278	2285	rVB	31085	39925	1.31%	0.232%
15	15.933	2349	2354	2360	rVB2	23569	35100	1.15%	0.204%
16	16.457	2437	2443	2452	rVB2	21747	37800	1.24%	0.219%
17	17.074	2543	2548	2556	rVB6	14386	30772	1.01%	0.179%




Sum of corrected areas: 17237165

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136655.D
Acq On : 20 Dec 2023 19:05
Operator : CG\JU
Sample : PB157610BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157610BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

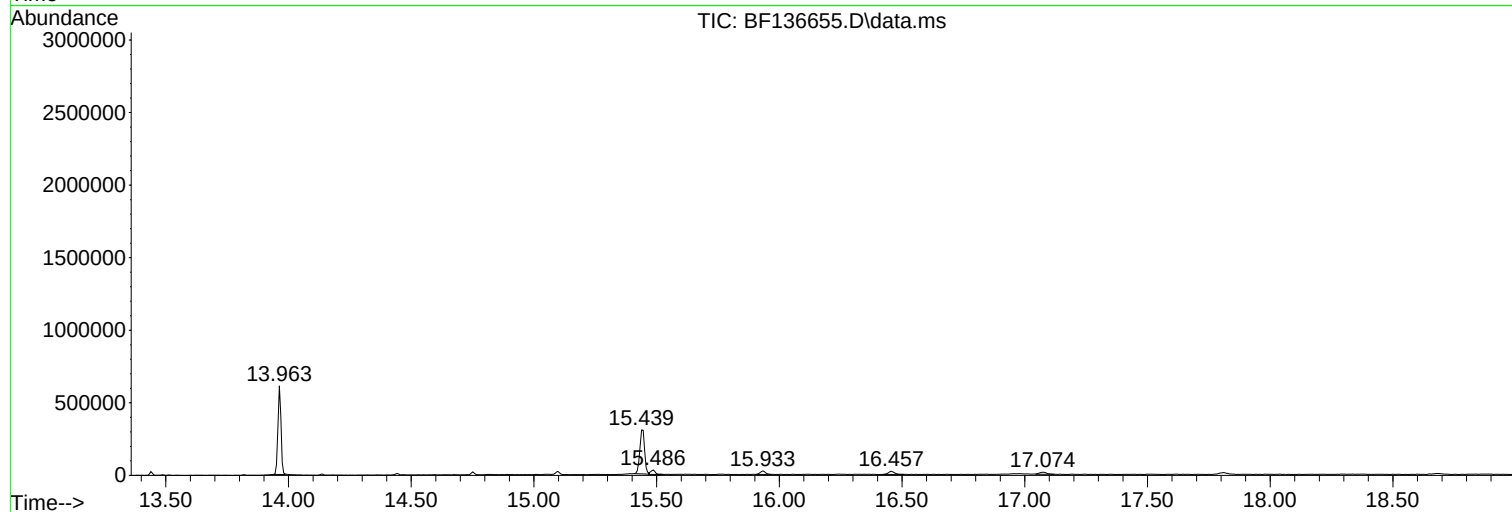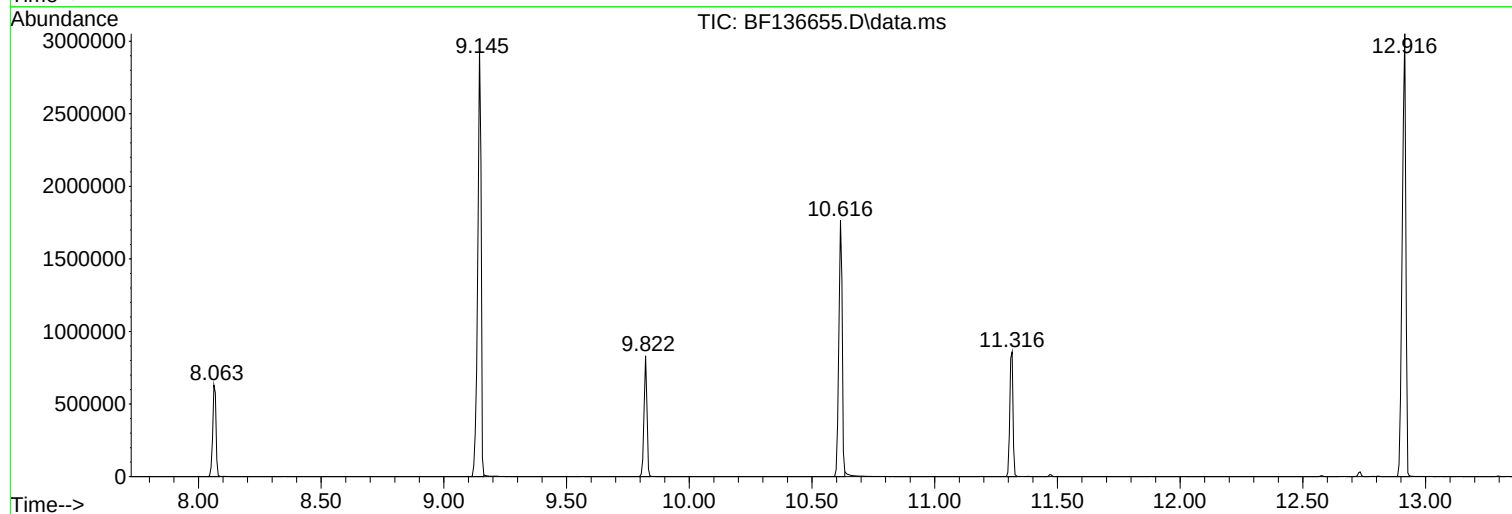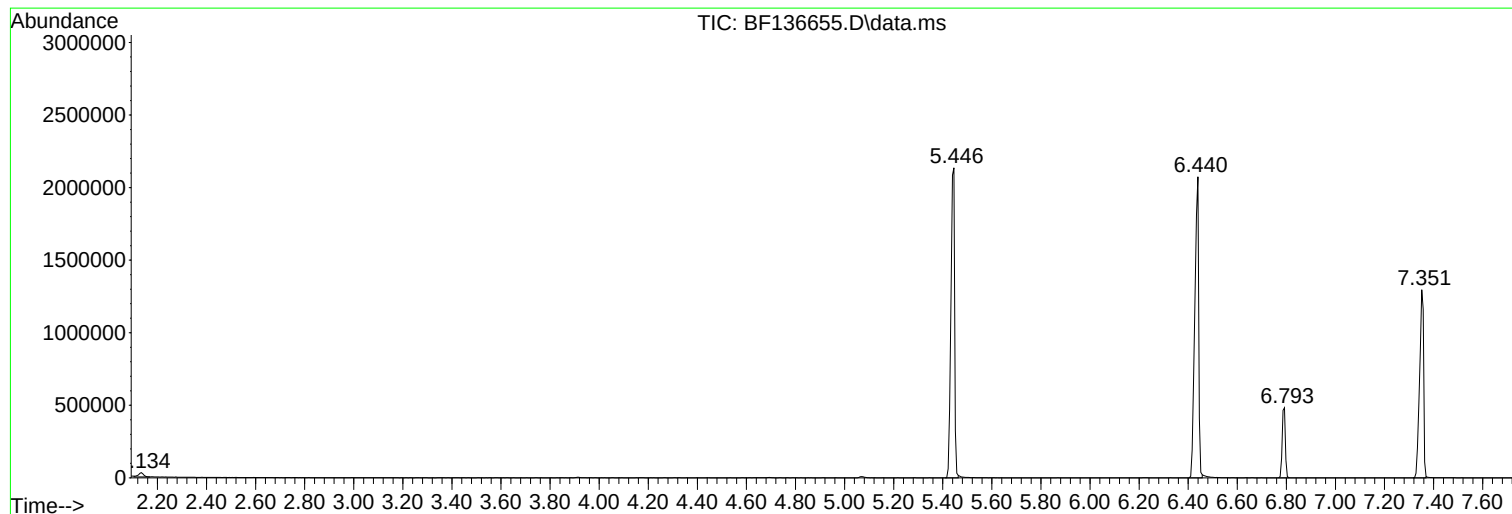

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136655.D
Acq On : 20 Dec 2023 19:05
Operator : CG\JU
Sample : PB157610BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157610BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136655.D
Acq On : 20 Dec 2023 19:05
Operator : CG\JU
Sample : PB157610BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157610BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------