

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
 Data File : BF136658.D
 Acq On : 20 Dec 2023 20:40
 Operator : CG\JU
 Sample : PB157519BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157519BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.387	388	391	396	rBV	13400	14464	2.05%	0.324%
2	5.428	564	568	579	rBV	219030	217165	30.71%	4.862%
3	6.422	734	737	751	rBV	220044	222883	31.52%	4.990%
4	6.787	796	799	803	rBV	464980	401704	56.80%	8.993%
5	7.345	890	894	905	rVB	169285	143351	20.27%	3.209%
6	8.063	1012	1016	1020	rBV	647111	541306	76.54%	12.118%
7	9.139	1195	1199	1207	rBV	408685	315242	44.58%	7.057%
8	9.822	1311	1315	1318	rBV	787461	642468	90.85%	14.383%
9	10.610	1446	1449	1458	rBV	123796	108382	15.33%	2.426%
10	11.310	1564	1568	1572	rBV	820651	707201	100.00%	15.832%
11	12.904	1835	1839	1842	rBV	381403	306025	43.27%	6.851%
12	13.963	2015	2019	2028	rVB	516737	453348	64.10%	10.149%
13	15.439	2264	2270	2280	rBV	299862	382555	54.09%	8.564%
14	15.768	2320	2326	2329	rBV7	4977	10769	1.52%	0.241%




Sum of corrected areas: 4466863

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136658.D
Acq On : 20 Dec 2023 20:40
Operator : CG\JU
Sample : PB157519BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157519BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

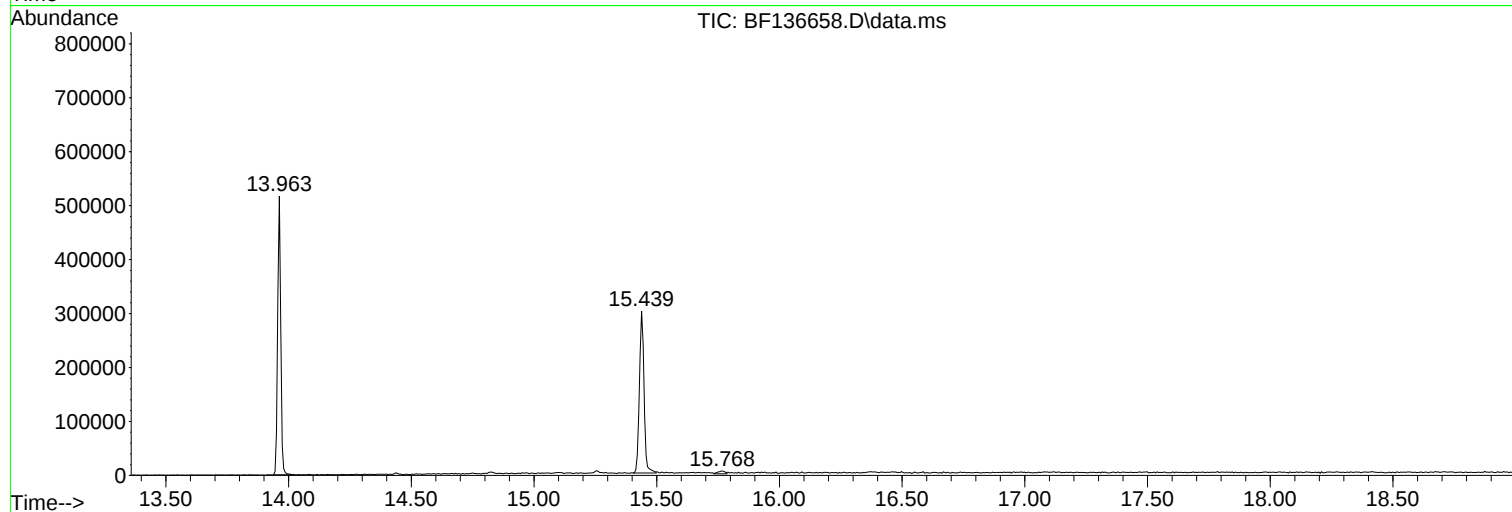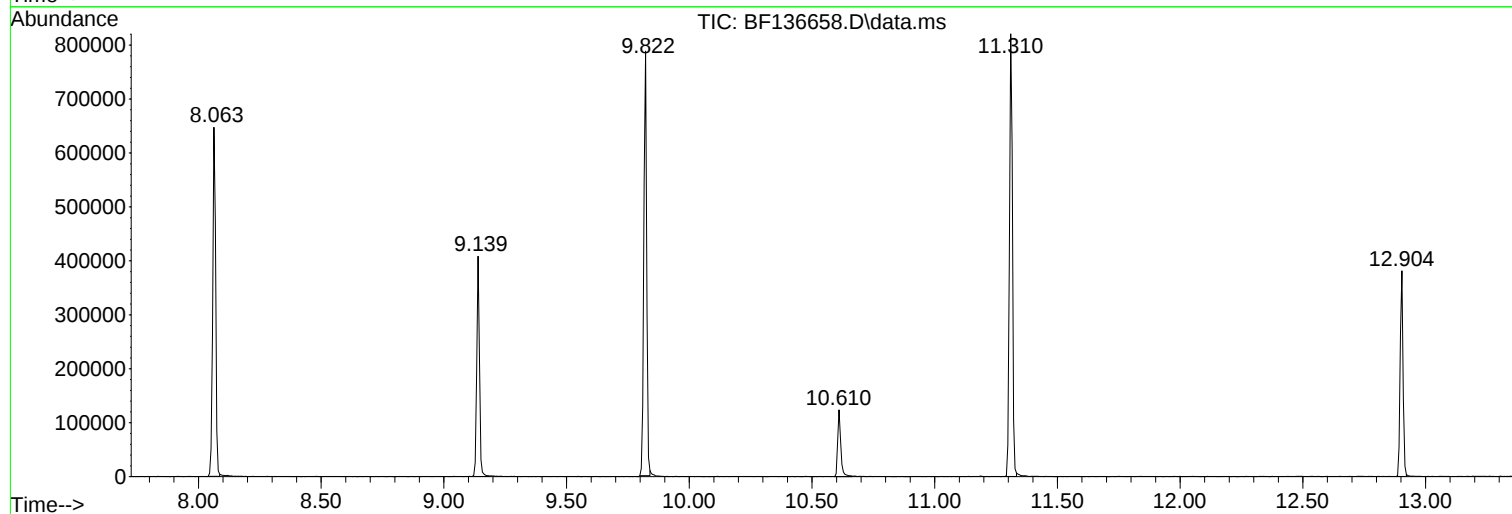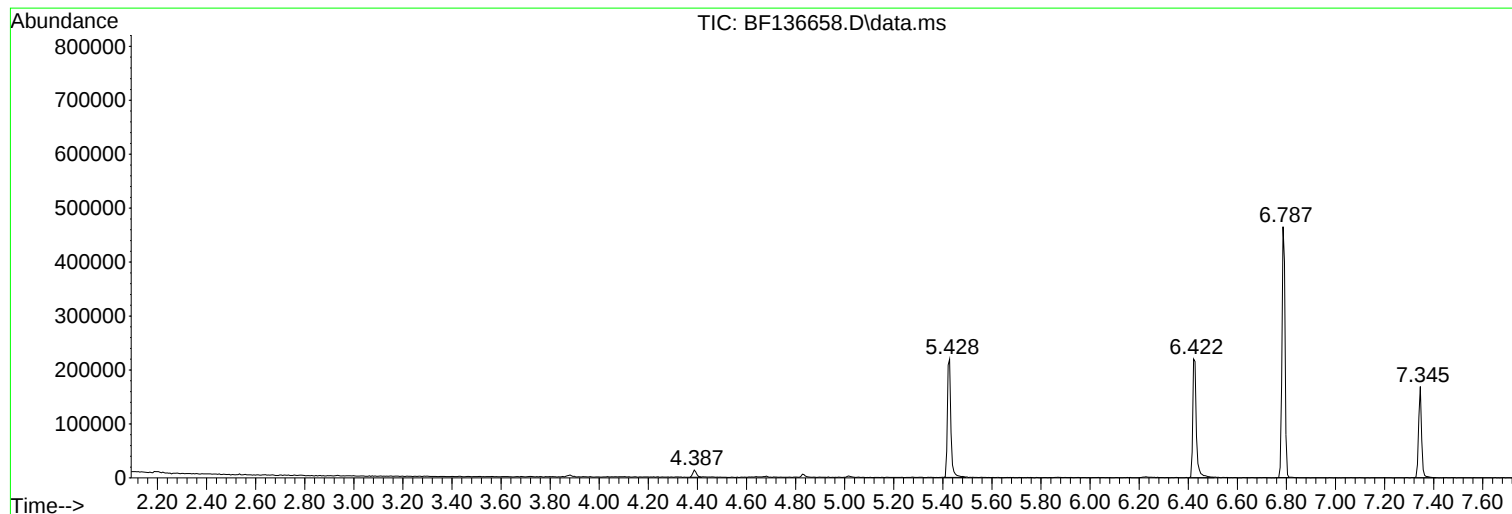

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136658.D
Acq On : 20 Dec 2023 20:40
Operator : CG\JU
Sample : PB157519BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157519BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136658.D
Acq On : 20 Dec 2023 20:40
Operator : CG\JU
Sample : PB157519BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157519BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------