
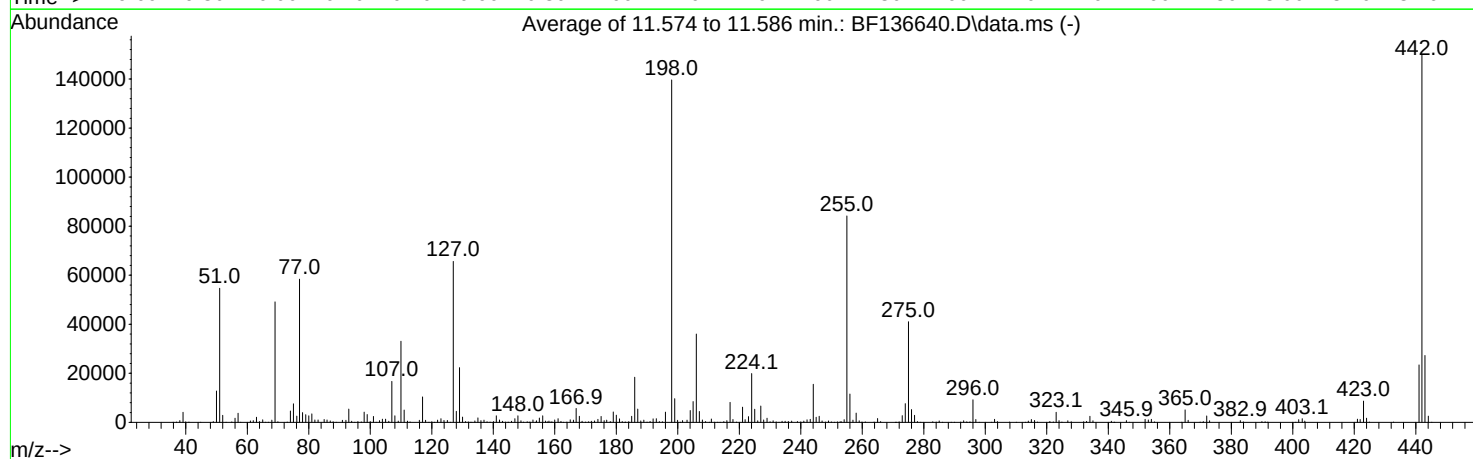


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
 Data File : BF136640.D
 Acq On : 20 Dec 2023 08:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 21 01:54:25 2023

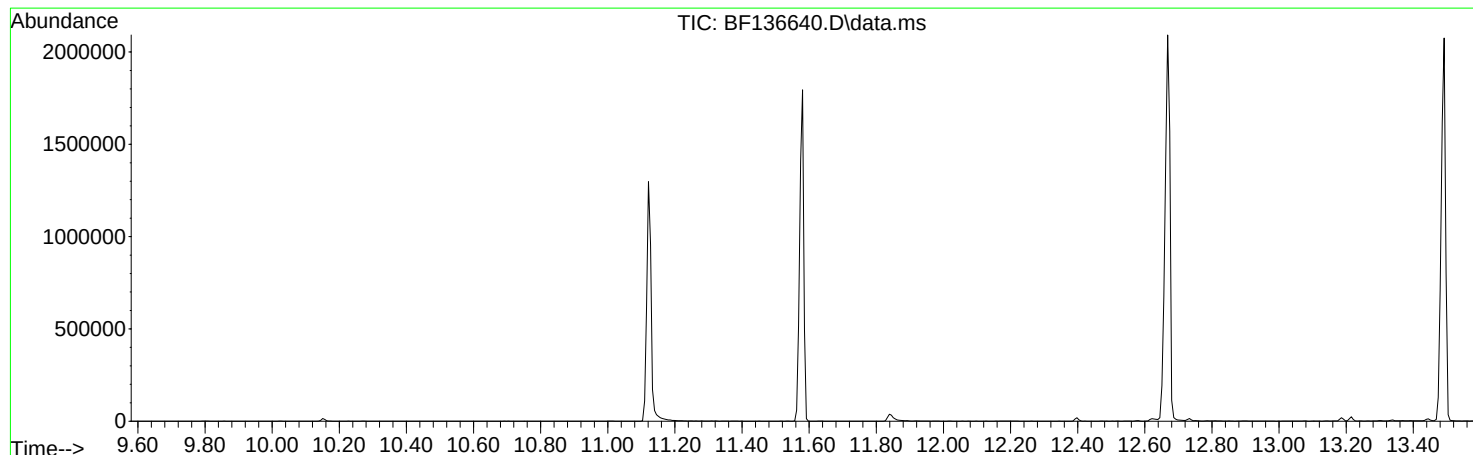




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	54672	PASS
68	69	0.00	2	1.8	888	PASS
69	198	0.00	100	35.2	49142	PASS
70	69	0.00	2	0.5	251	PASS
127	198	10	80	47.0	65659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139621	PASS
199	198	5	9	6.9	9654	PASS
275	198	10	60	29.4	41061	PASS
365	198	1	100	3.7	5100	PASS
441	198	0.01	100	16.8	23435	PASS
442	442	50	100	100.0	150005	PASS
443	442	15	24	18.2	27264	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136640.D
Acq On : 20 Dec 2023 08:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 16:17:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 15:40:36 2023
Response via : Initial Calibration

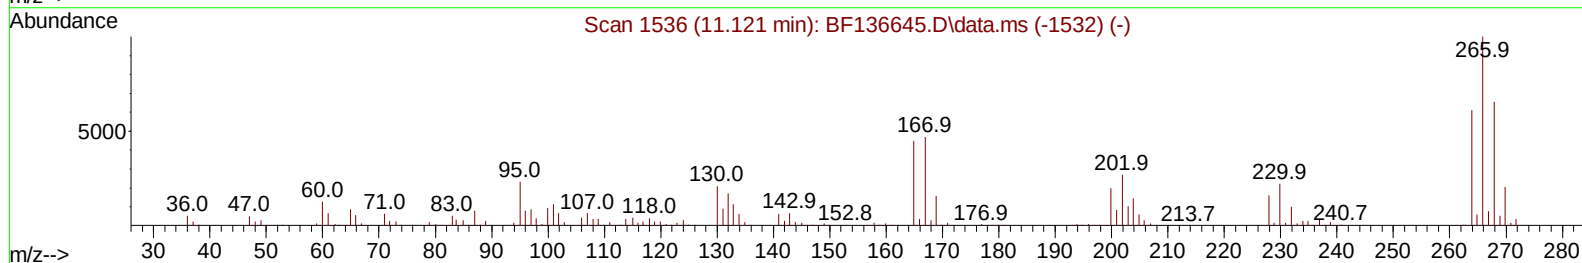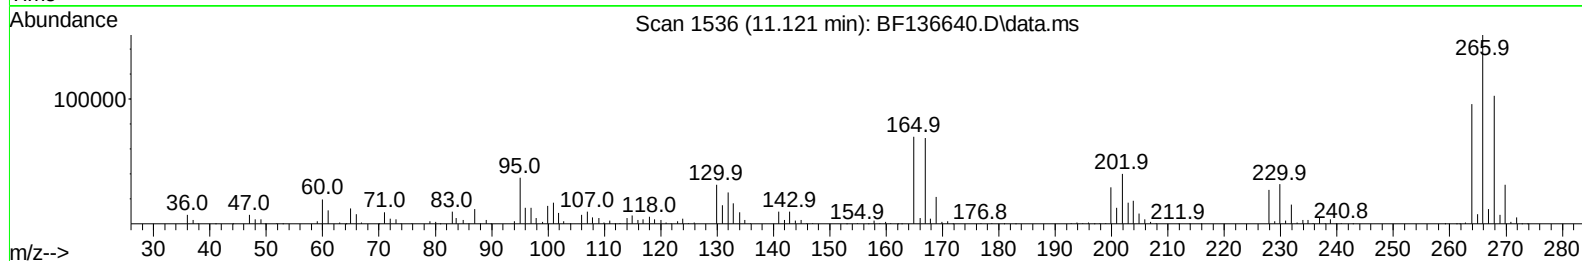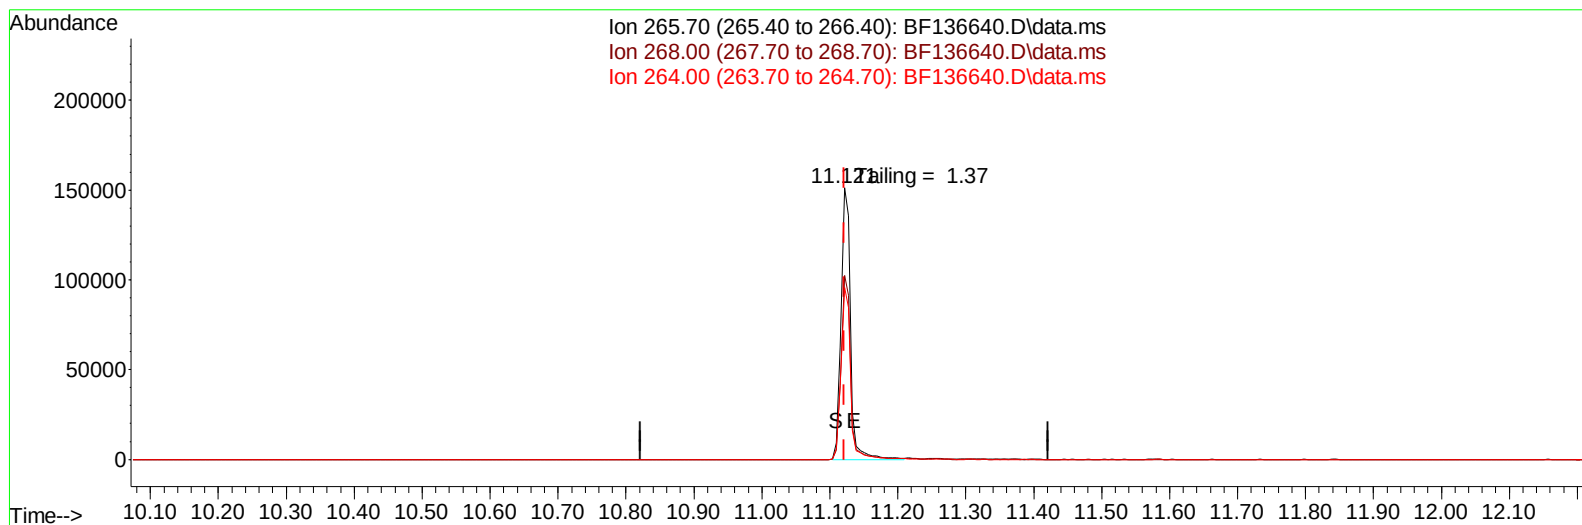

TIC: BF136640.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.000) 35779.06 ng




response 146132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.69
264.00	61.20	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122023\
Data File : BF136640.D
Acq On : 20 Dec 2023 08:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 16:17:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 15:40:36 2023
Response via : Initial Calibration

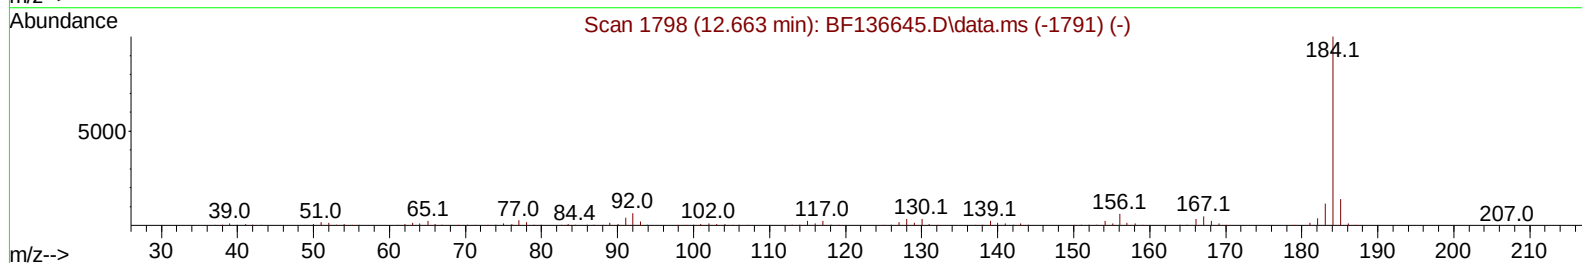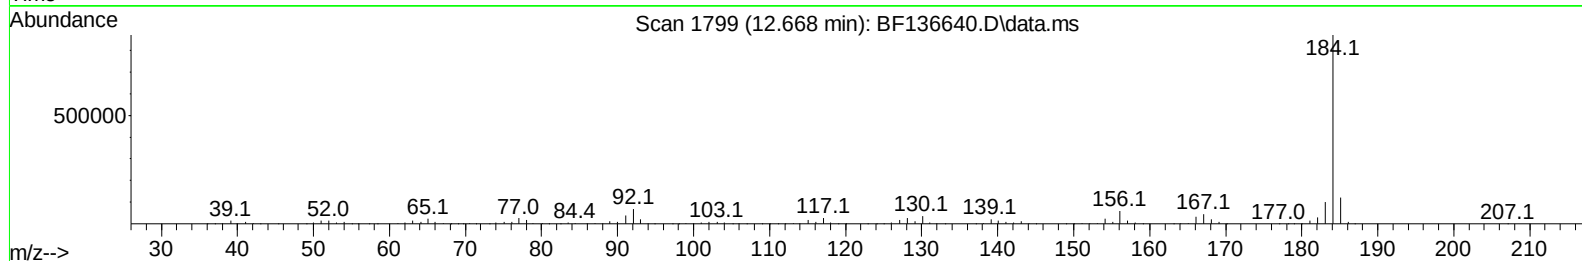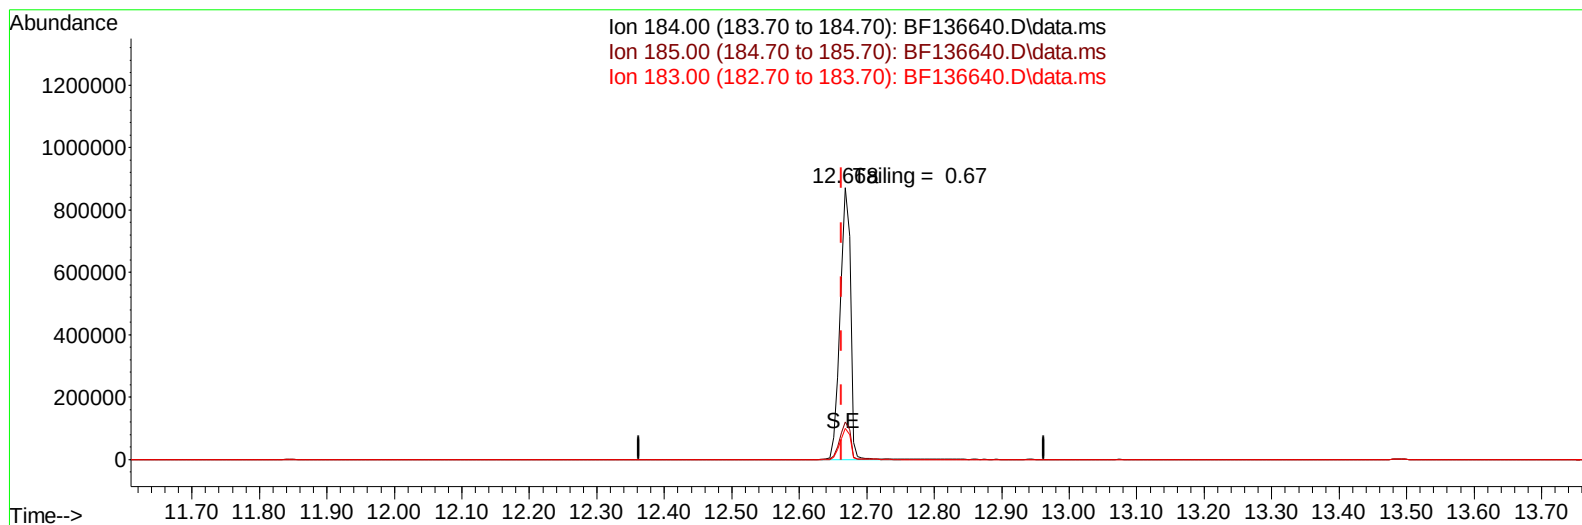

TIC: BF136640.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 0.00 ng

response 918090

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.85
183.00	11.60	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2023	BNA_F	<u>BF136640.D</u>
Compound Name	Response	Retention Time
DDT	392773	13.492
DDD	7855	13.216
DDE	0	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7855	400628	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP