
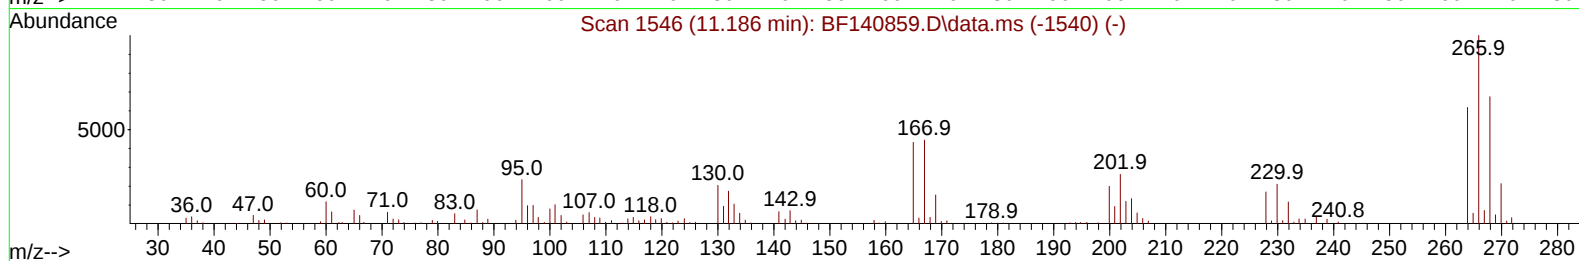
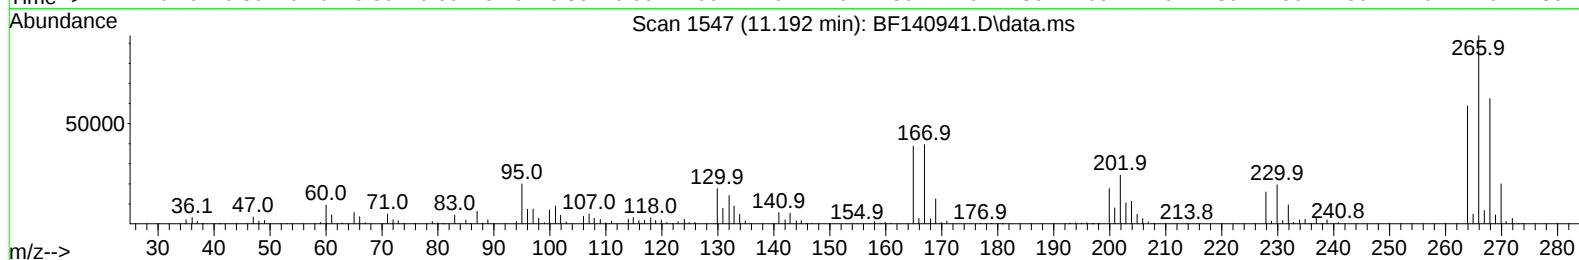


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140941.D
Acq On : 20 Dec 2024 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 11:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

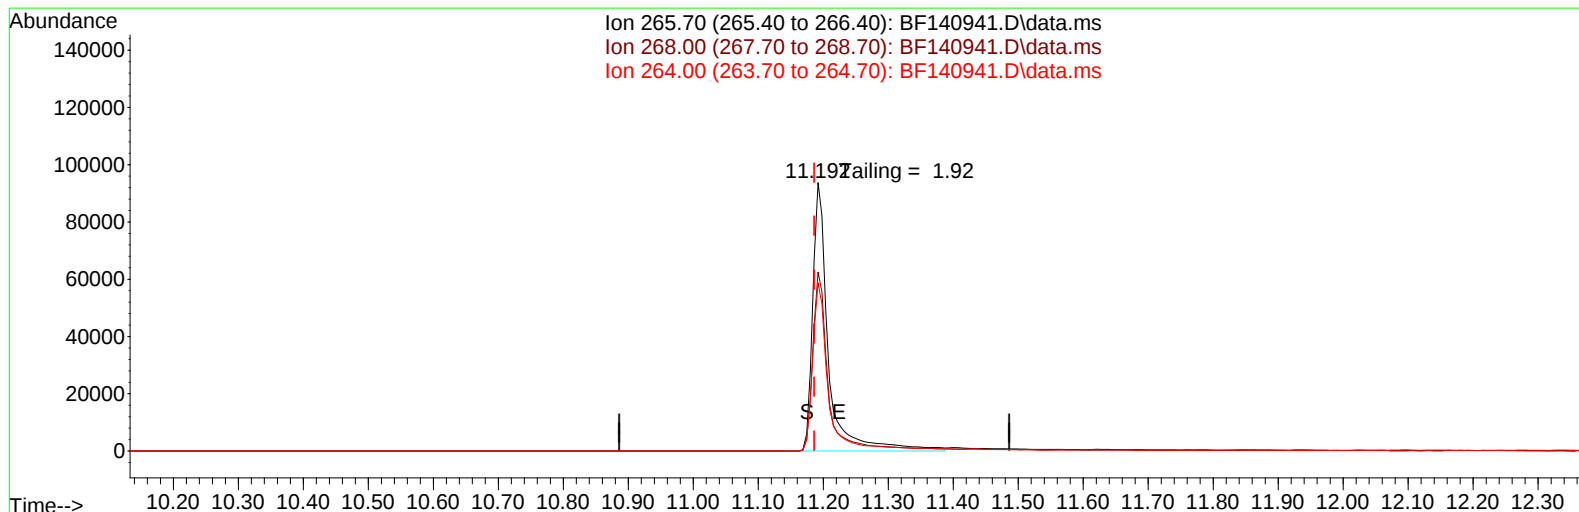

TIC: BF140941.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.006) 18269.88 ng

response 157756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	66.64
264.00	61.80	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140941.D
Acq On : 20 Dec 2024 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 11:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

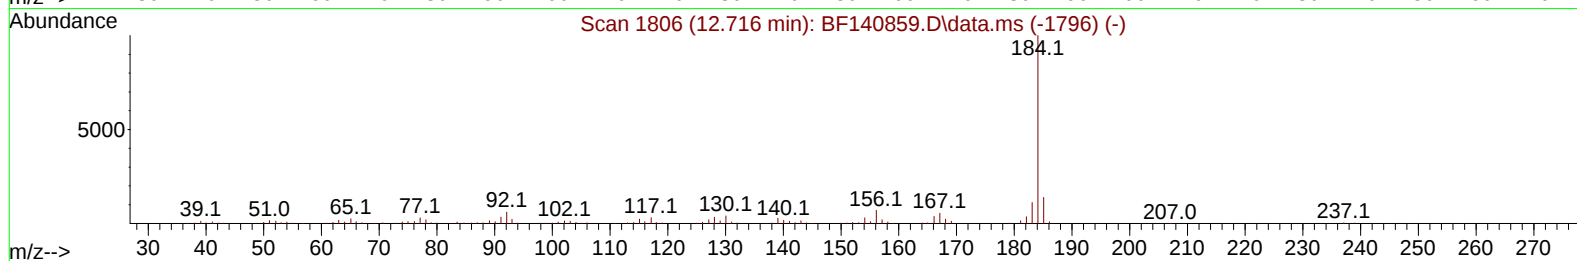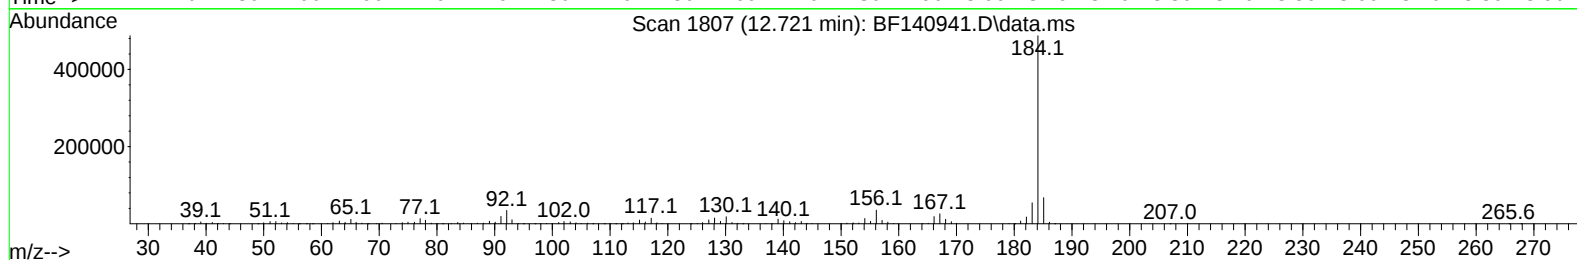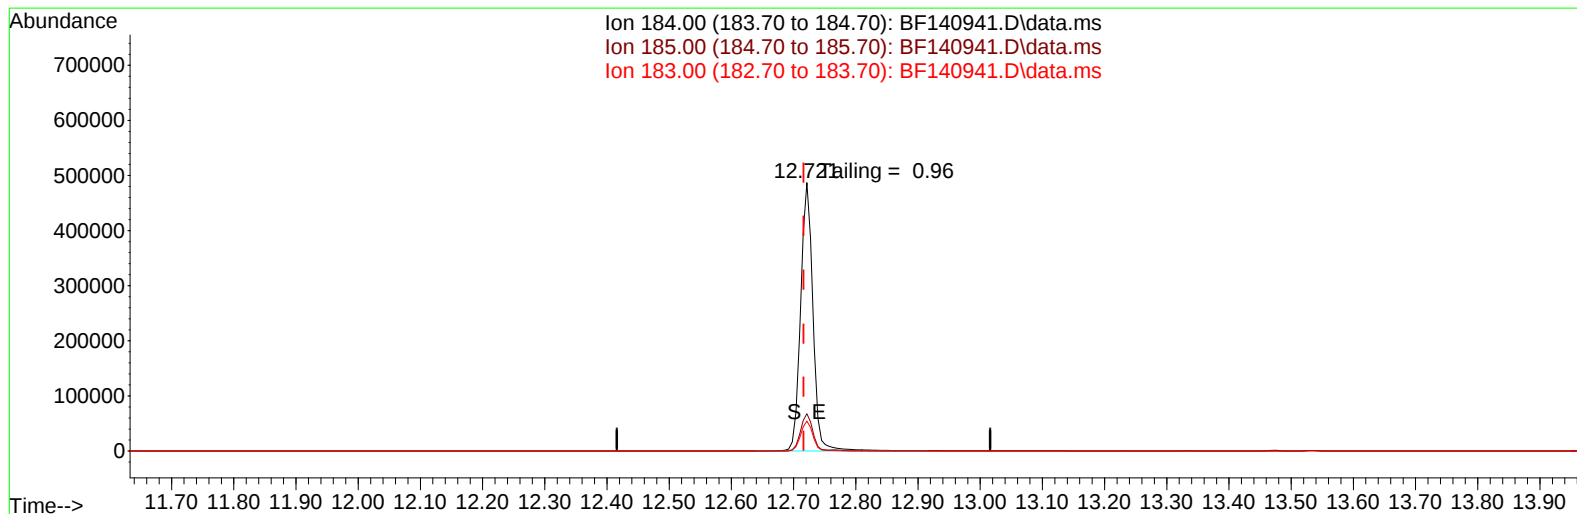

TIC: BF140941.D\data.ms

(77) Benzidine

12.721min (+ 0.005) 28215.57 ng

response 676070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.93
183.00	11.20	11.19
0.00	0.00	0.00