

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140946.D
 Acq On : 20 Dec 2024 13:18
 Operator : RC/JU
 Sample : P5306-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-12-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	3	14	27	rVB	1222430	2089275	87.49%	12.777%
2	5.104	507	512	527	rVB	18900	35686	1.49%	0.218%
3	5.498	574	579	606	rBV	1269209	1817451	76.11%	11.115%
4	6.504	744	750	782	rBV	1336136	1982021	83.00%	12.121%
5	6.845	804	808	817	rVB	234349	301726	12.64%	1.845%
6	7.416	899	905	929	rBV	884244	1211297	50.72%	7.408%
7	7.669	944	948	961	rBV	18520	32360	1.36%	0.198%
8	8.128	1021	1026	1039	rBV	304991	404455	16.94%	2.473%
9	9.204	1202	1209	1218	rBV	1734350	2300806	96.35%	14.071%
10	9.886	1319	1325	1338	rBV	359655	483615	20.25%	2.958%
11	10.598	1441	1446	1455	rBV	223541	281103	11.77%	1.719%
12	10.681	1455	1460	1483	rVV	1064215	1457202	61.02%	8.912%
13	11.375	1573	1578	1586	rBV	369339	495489	20.75%	3.030%
14	11.898	1662	1667	1690	rBV	93258	169745	7.11%	1.038%
15	12.680	1794	1800	1812	rBV2	12554	28983	1.21%	0.177%
16	12.963	1842	1848	1853	rBV	1804927	2388001	100.00%	14.604%
17	13.857	1994	2000	2018	rBV2	52266	142566	5.97%	0.872%
18	14.027	2024	2029	2040	rBV	306654	424029	17.76%	2.593%
19	15.527	2278	2284	2298	rVB	168249	306045	12.82%	1.872%




Sum of corrected areas: 16351855

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140946.D
Acq On : 20 Dec 2024 13:18
Operator : RC/JU
Sample : P5306-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-12-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

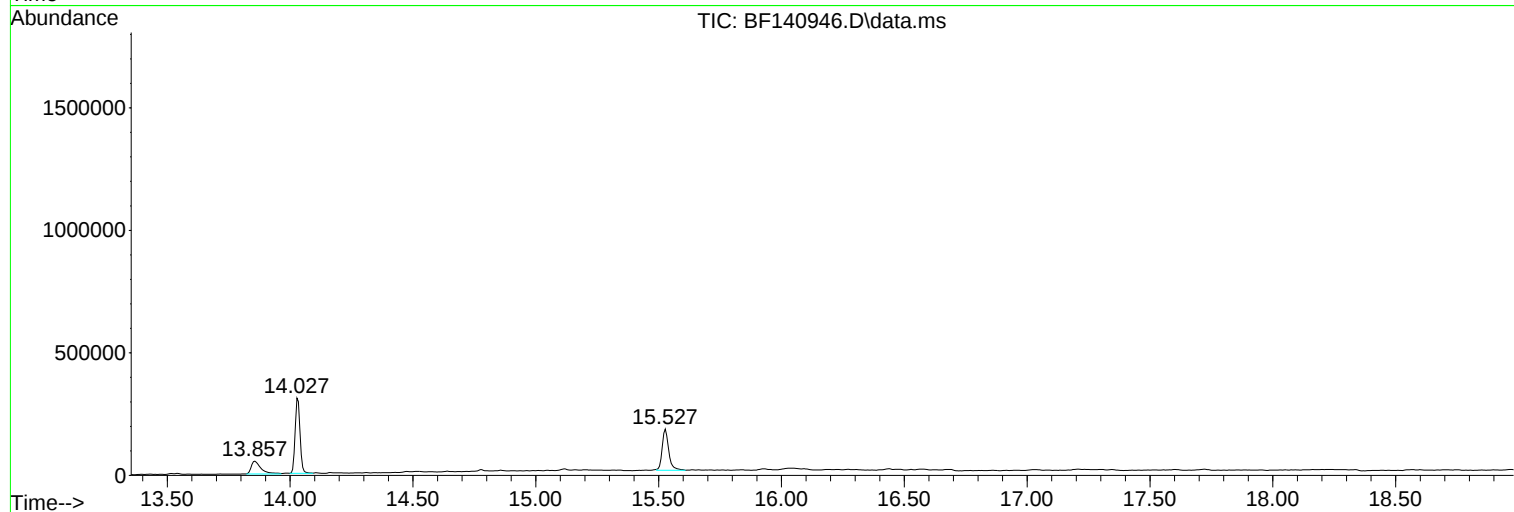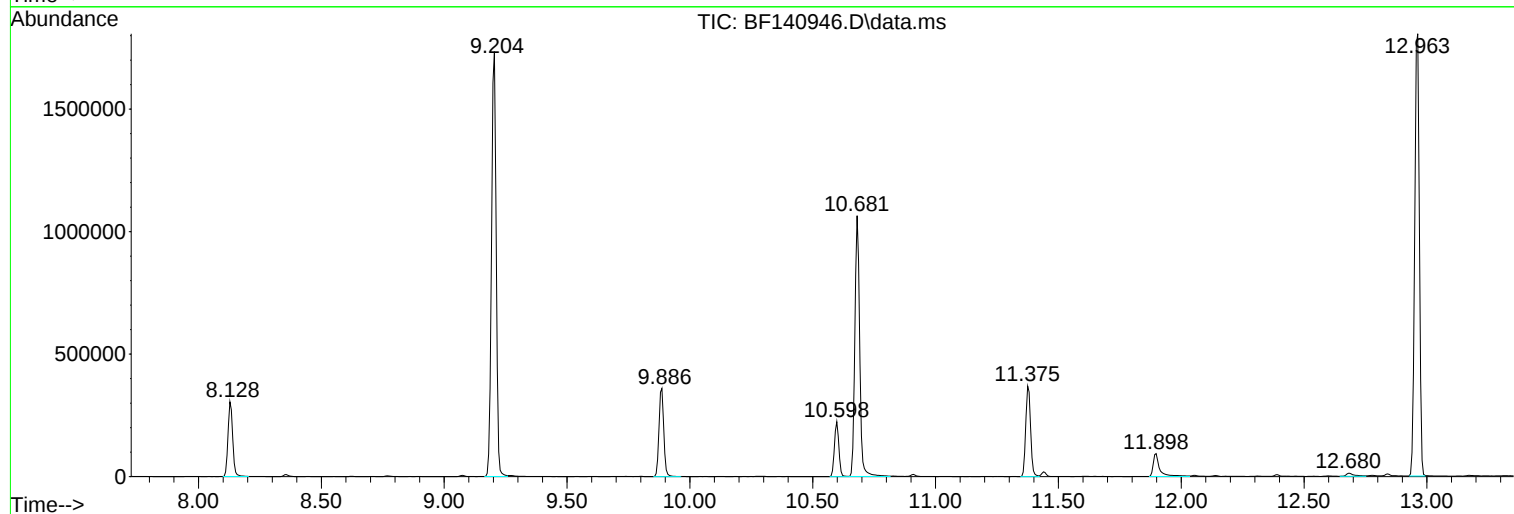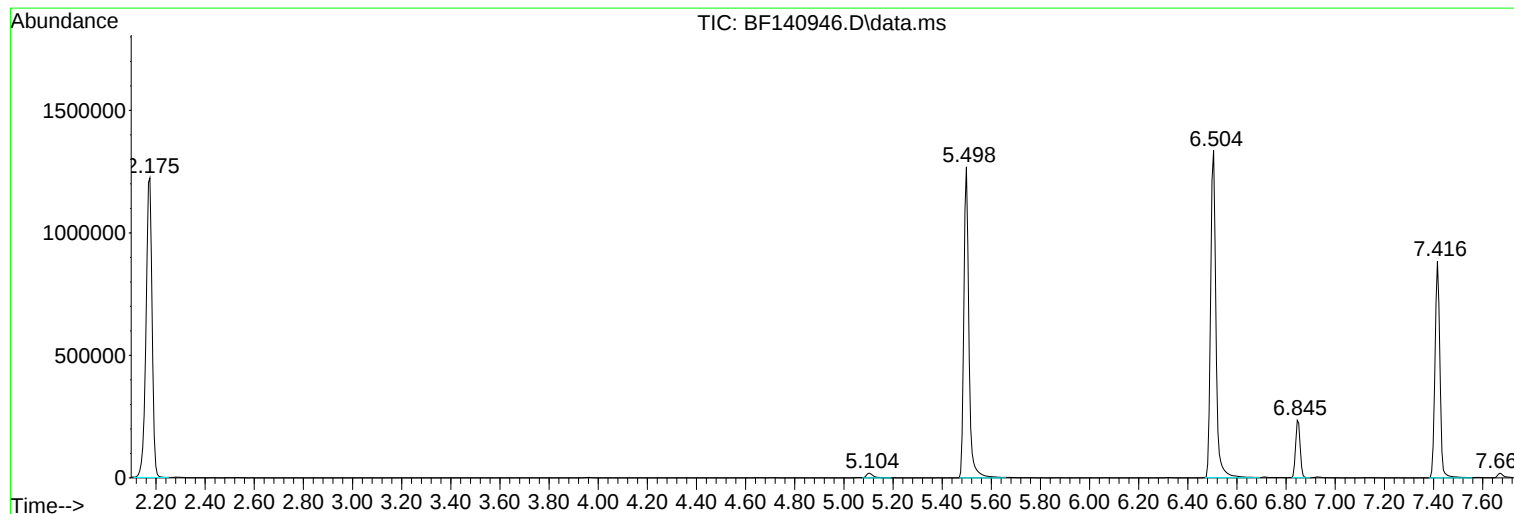

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140946.D
Acq On : 20 Dec 2024 13:18
Operator : RC/JU
Sample : P5306-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-12-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140946.D
Acq On : 20 Dec 2024 13:18
Operator : RC/JU
Sample : P5306-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-12-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------