

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140947.D
 Acq On : 20 Dec 2024 13:44
 Operator : RC/JU
 Sample : P5306-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-11-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	3	10	20	rVB	1047168	1670768	93.36%	12.876%
2	5.493	573	578	607	rBV	825017	1261115	70.47%	9.719%
3	6.498	744	749	778	rBV	917508	1405301	78.52%	10.830%
4	6.846	804	808	816	rVB	255112	328162	18.34%	2.529%
5	7.416	899	905	925	rBV	673485	909472	50.82%	7.009%
6	7.675	945	949	960	rBV	10824	21287	1.19%	0.164%
7	8.128	1021	1026	1046	rBV	318215	421656	23.56%	3.249%
8	9.198	1203	1208	1218	rBV	1336170	1789661	100.00%	13.792%
9	9.881	1319	1324	1346	rVB	354775	489190	27.33%	3.770%
10	10.598	1441	1446	1455	rBV	180743	235221	13.14%	1.813%
11	10.681	1455	1460	1484	rVV	777965	1073534	59.99%	8.273%
12	10.904	1494	1498	1508	rVB	11977	17969	1.00%	0.138%
13	11.375	1573	1578	1586	rBV	454137	595685	33.28%	4.591%
14	11.439	1586	1589	1594	rVB	14860	18477	1.03%	0.142%
15	11.892	1661	1666	1679	rBV2	45204	81736	4.57%	0.630%
16	12.957	1842	1847	1858	rBV	1353572	1755693	98.10%	13.530%
17	13.857	1993	2000	2017	rBV2	34284	97652	5.46%	0.753%
18	14.027	2024	2029	2038	rBV	341482	464310	25.94%	3.578%
19	15.521	2277	2283	2300	rVB	188944	339296	18.96%	2.615%




Sum of corrected areas: 12976185

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140947.D
Acq On : 20 Dec 2024 13:44
Operator : RC/JU
Sample : P5306-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-11-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

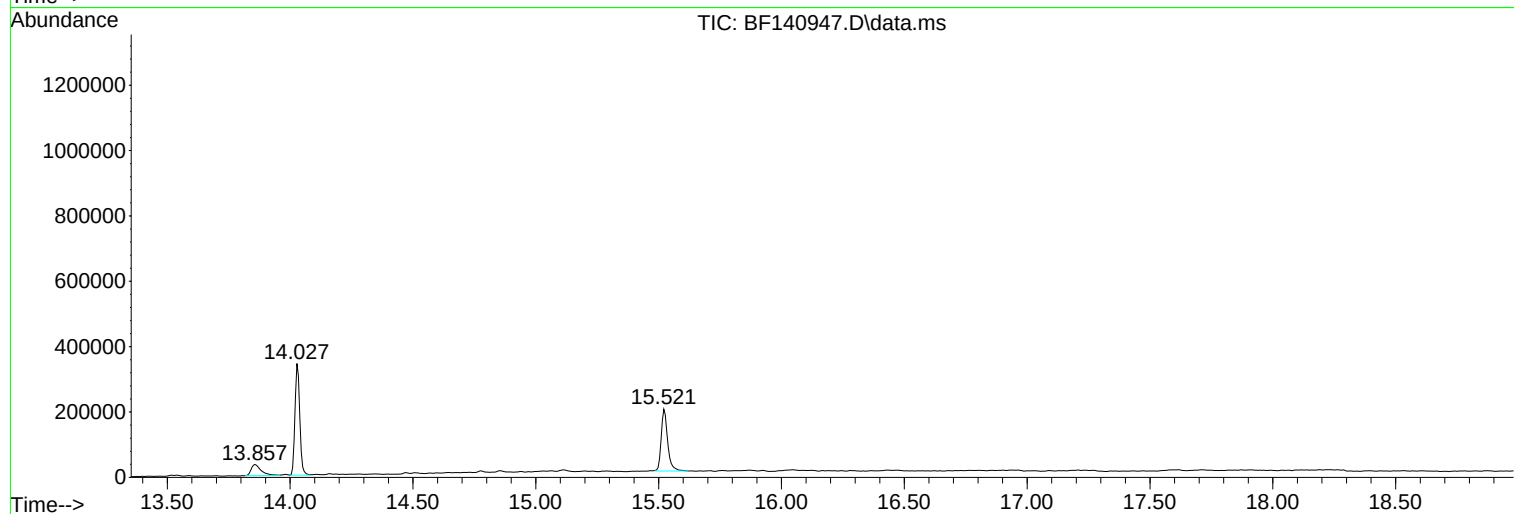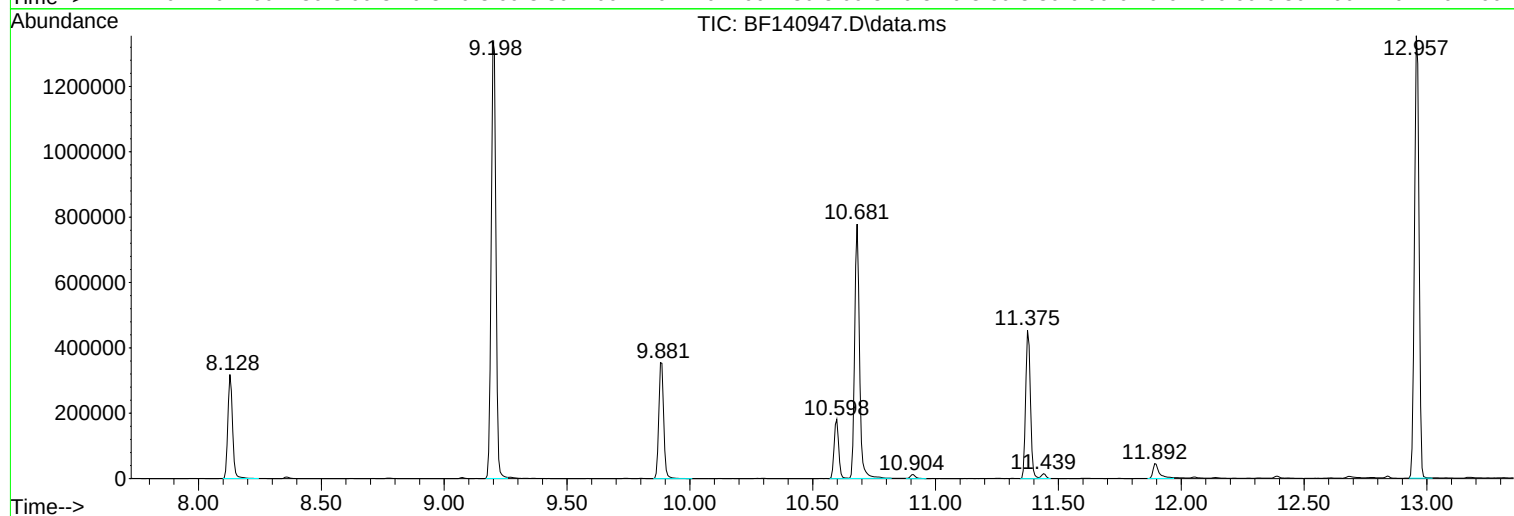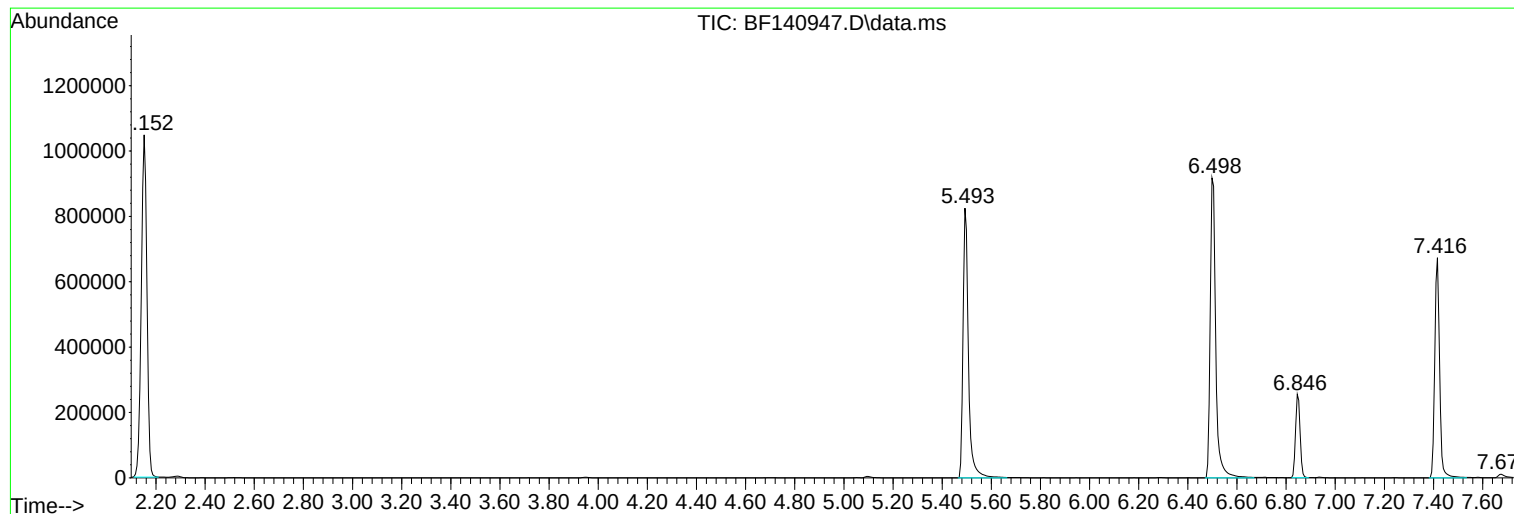

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140947.D
Acq On : 20 Dec 2024 13:44
Operator : RC/JU
Sample : P5306-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-11-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140947.D
Acq On : 20 Dec 2024 13:44
Operator : RC/JU
Sample : P5306-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-11-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------