

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140950.D
 Acq On : 20 Dec 2024 15:02
 Operator : RC/JU
 Sample : P5306-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-13-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	3	12	28	rVB	1136340	1905688	78.77%	11.964%
2	5.498	573	579	606	rBV	1147349	1689777	69.84%	10.608%
3	6.504	744	750	775	rBV	1242966	1832273	75.73%	11.503%
4	6.845	803	808	815	rBV	238120	302576	12.51%	1.900%
5	7.416	899	905	923	rBV	890652	1218854	50.38%	7.652%
6	7.669	942	948	964	rBV	18983	34671	1.43%	0.218%
7	8.128	1021	1026	1051	rVB	315732	415894	17.19%	2.611%
8	9.204	1202	1209	1218	rBV	1747546	2289533	94.63%	14.373%
9	9.886	1319	1325	1338	rBV	364551	494871	20.45%	3.107%
10	10.598	1441	1446	1455	rBV	233118	294353	12.17%	1.848%
11	10.680	1455	1460	1474	rBV	1040730	1406009	58.12%	8.827%
12	11.374	1573	1578	1586	rBV	388524	520866	21.53%	3.270%
13	11.898	1662	1667	1682	rBV	81320	144447	5.97%	0.907%
14	12.680	1796	1800	1812	rBV2	11588	25331	1.05%	0.159%
15	12.963	1842	1848	1853	rBV	1828354	2419334	100.00%	15.188%
16	13.857	1994	2000	2018	rBV2	53225	149918	6.20%	0.941%
17	14.033	2025	2030	2040	rBV	309099	431654	17.84%	2.710%
18	15.545	2282	2287	2301	rVB	197697	352906	14.59%	2.216%




Sum of corrected areas: 15928955

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140950.D
Acq On : 20 Dec 2024 15:02
Operator : RC/JU
Sample : P5306-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-13-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

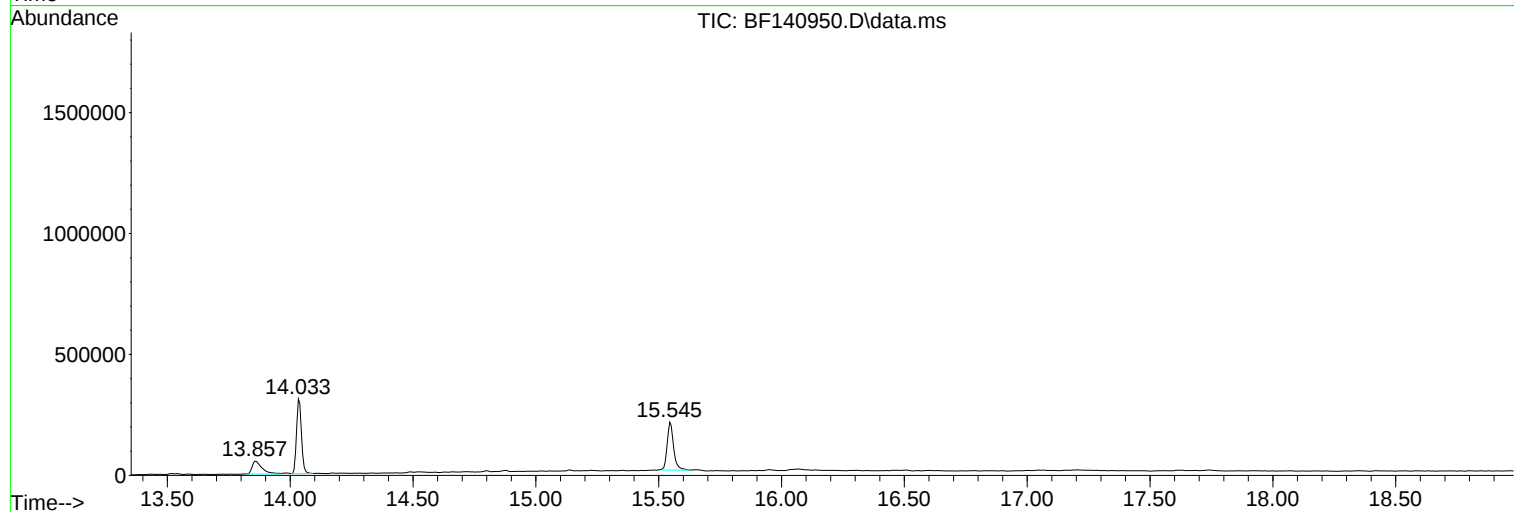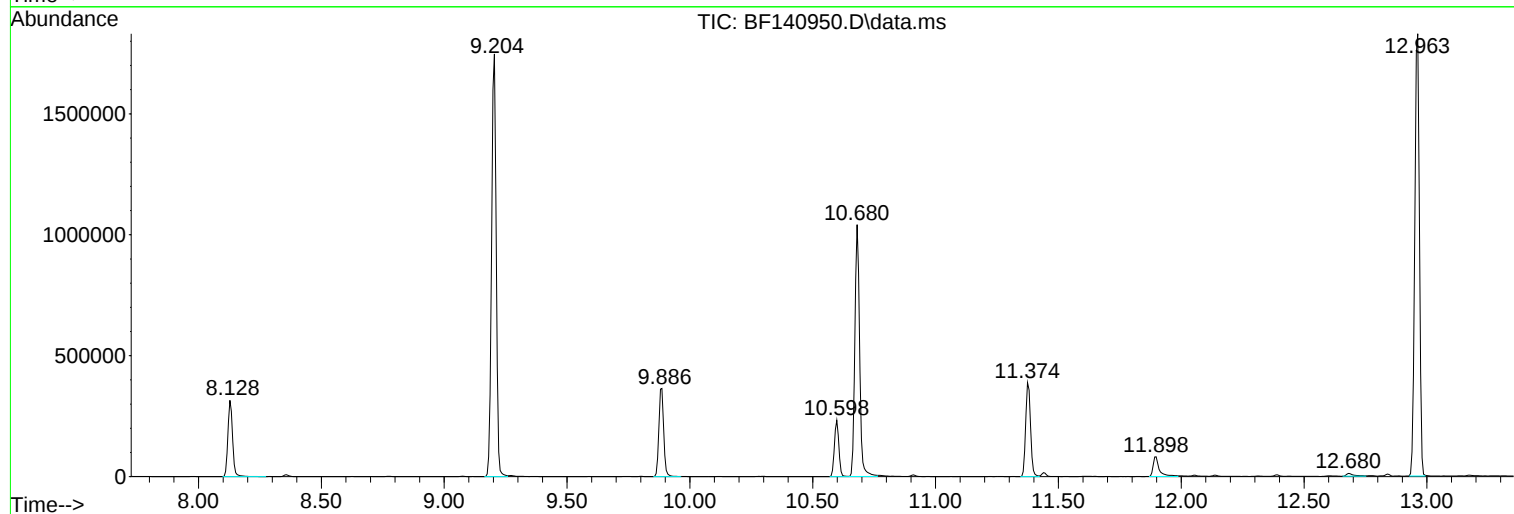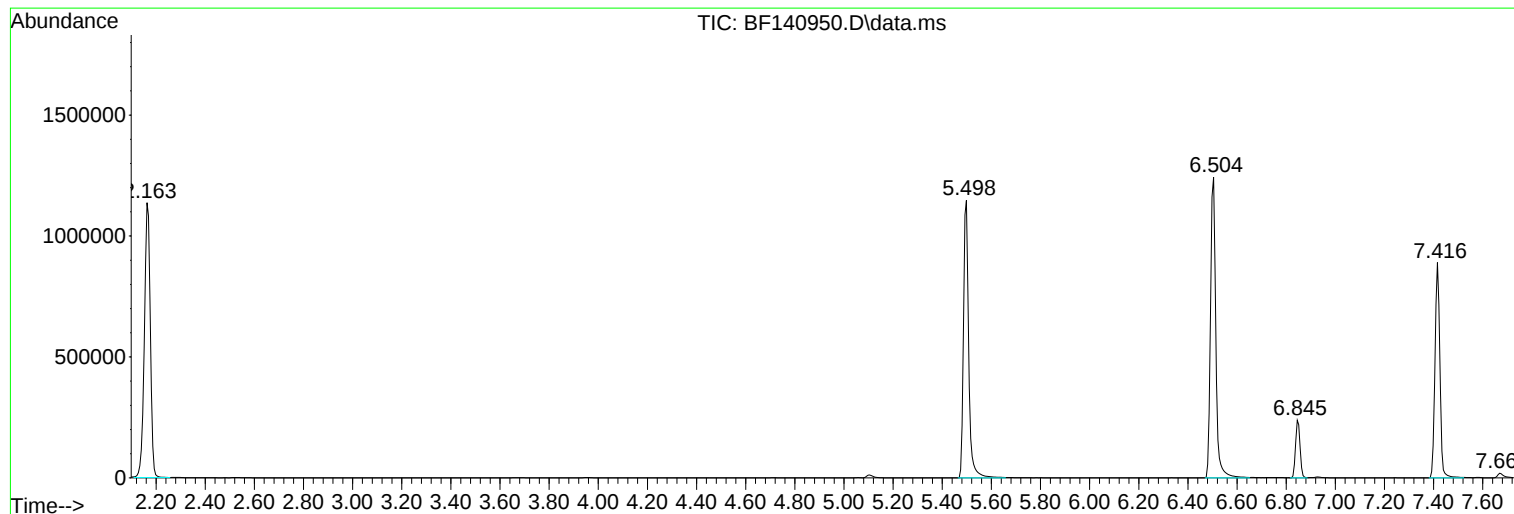

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140950.D
Acq On : 20 Dec 2024 15:02
Operator : RC/JU
Sample : P5306-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-13-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140950.D
Acq On : 20 Dec 2024 15:02
Operator : RC/JU
Sample : P5306-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-13-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------