

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140951.D
 Acq On : 20 Dec 2024 15:29
 Operator : RC/JU
 Sample : P5306-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-14-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	3	12	28	rVB	1232008	2069517	64.83%	11.480%
2	5.498	573	579	609	rBV	1206150	1778749	55.72%	9.867%
3	6.504	744	750	783	rBV	1313007	1942755	60.86%	10.777%
4	6.845	804	808	817	rVB	221138	285509	8.94%	1.584%
5	7.416	899	905	924	rBV	915180	1271965	39.85%	7.056%
6	7.669	944	948	962	rBV	23594	38032	1.19%	0.211%
7	8.128	1021	1026	1043	rVB	300715	397849	12.46%	2.207%
8	9.204	1202	1209	1218	rBV	1984076	2673805	83.77%	14.832%
9	9.880	1319	1324	1339	rBV	362993	485245	15.20%	2.692%
10	10.598	1440	1446	1455	rBV	310104	390852	12.24%	2.168%
11	10.680	1455	1460	1483	rBV	1233248	1682257	52.70%	9.332%
12	11.374	1573	1578	1585	rBV	413026	541693	16.97%	3.005%
13	11.898	1662	1667	1680	rBV	132937	218081	6.83%	1.210%
14	12.680	1795	1800	1811	rBV	25296	51055	1.60%	0.283%
15	12.963	1842	1848	1853	rBV	2386314	3192017	100.00%	17.707%
16	13.863	1994	2001	2020	rBV	67578	187705	5.88%	1.041%
17	14.039	2026	2031	2042	rBV	340781	469904	14.72%	2.607%
18	15.557	2280	2289	2303	rBV	181670	349746	10.96%	1.940%




Sum of corrected areas: 18026736

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140951.D
Acq On : 20 Dec 2024 15:29
Operator : RC/JU
Sample : P5306-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-14-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

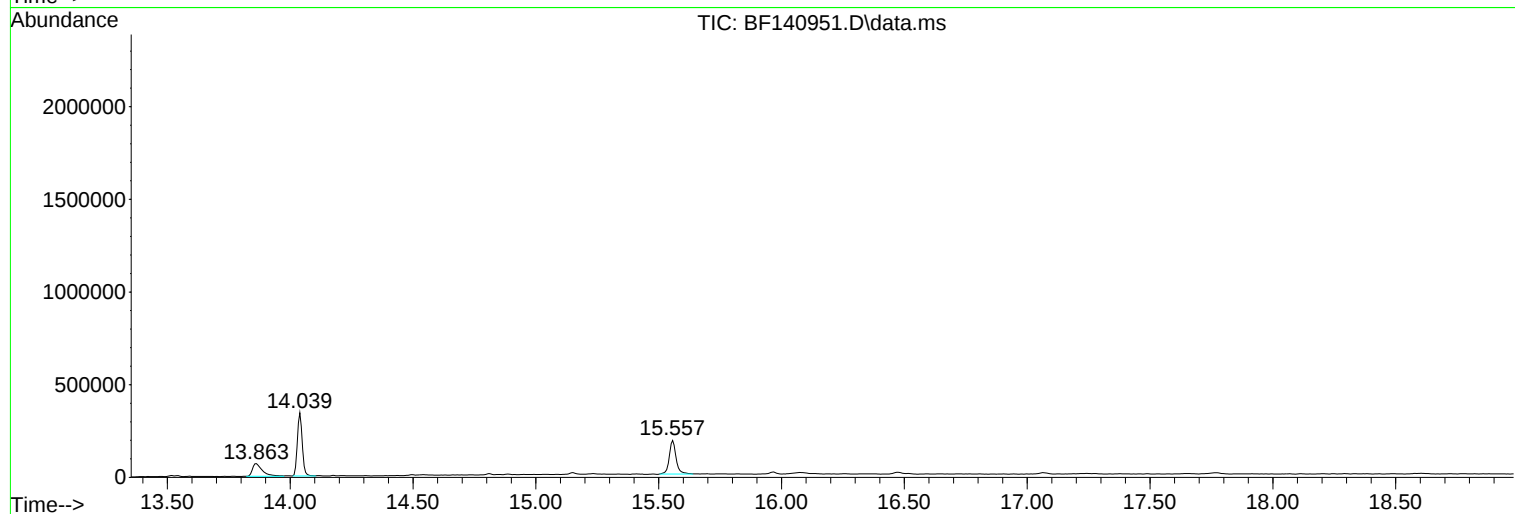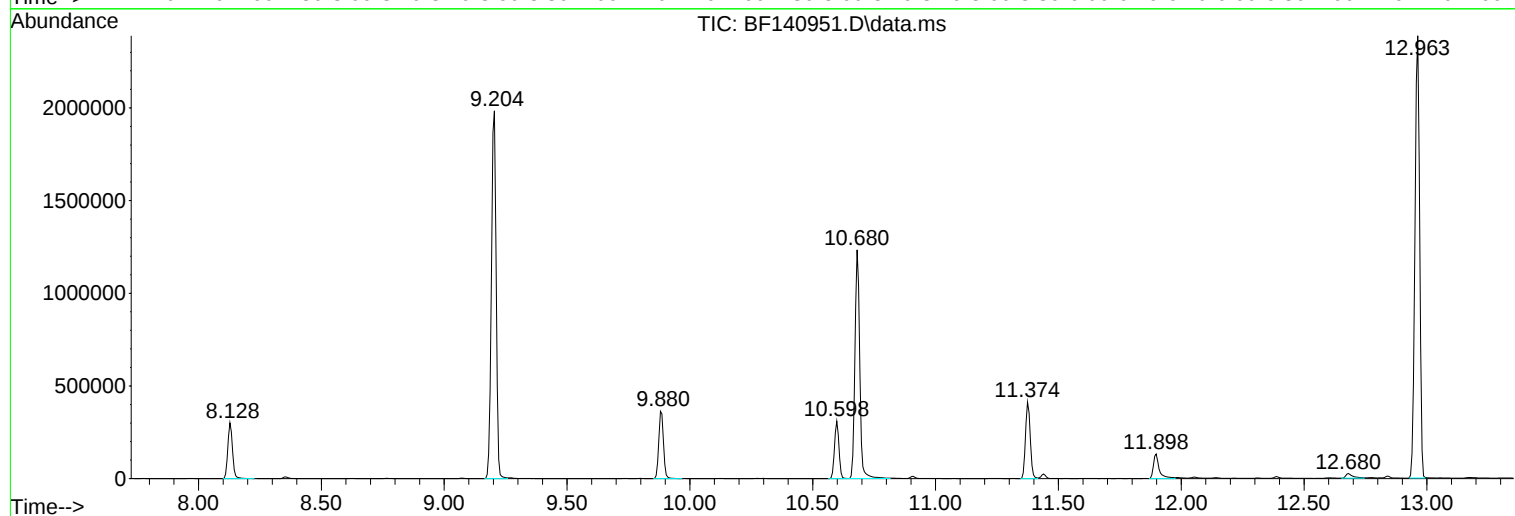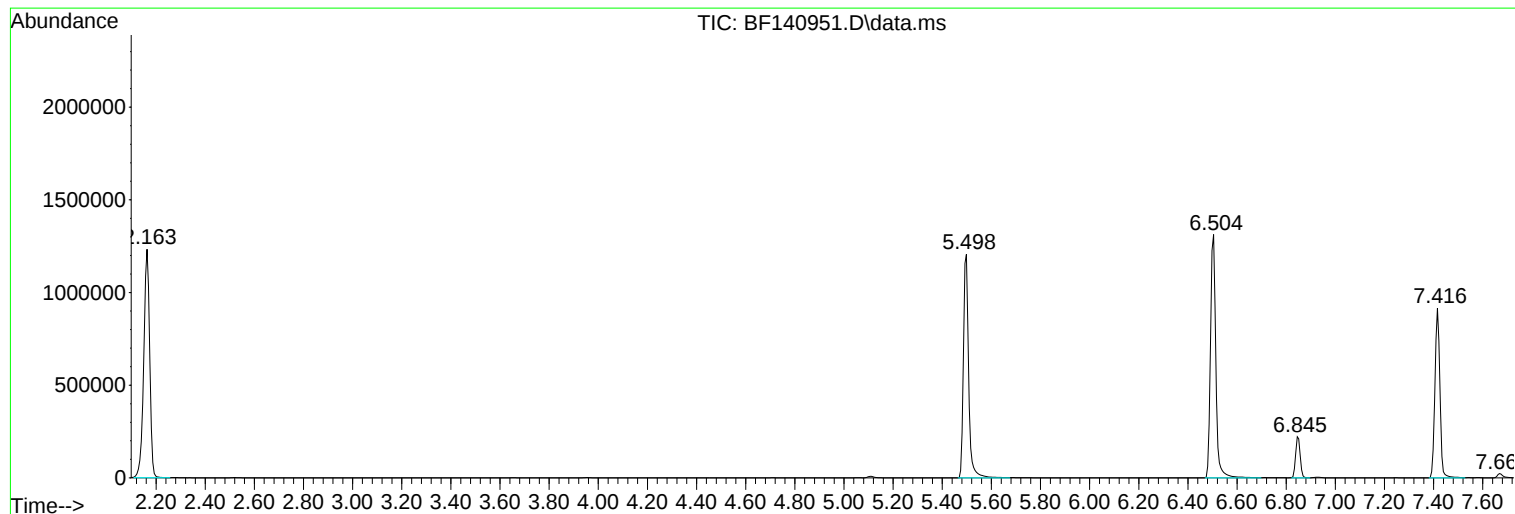

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140951.D
Acq On : 20 Dec 2024 15:29
Operator : RC/JU
Sample : P5306-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-14-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140951.D
Acq On : 20 Dec 2024 15:29
Operator : RC/JU
Sample : P5306-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-14-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------