

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140952.D
 Acq On : 20 Dec 2024 15:55
 Operator : RC/JU
 Sample : P5306-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-07-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	7	24	rVB	763762	1203878	80.80%	11.540%
2	5.493	573	578	609	rBV	613883	957031	64.23%	9.174%
3	6.498	744	749	781	rBV	676047	1034973	69.46%	9.921%
4	6.845	804	808	821	rBV	209380	267745	17.97%	2.567%
5	7.416	899	905	929	rBV	472788	656332	44.05%	6.292%
6	7.675	943	949	958	rBV2	8036	16120	1.08%	0.155%
7	8.128	1021	1026	1051	rBV	266076	356032	23.90%	3.413%
8	9.198	1203	1208	1227	rBV	1047125	1366258	91.70%	13.097%
9	9.881	1319	1324	1340	rBV	322020	439156	29.47%	4.210%
10	10.598	1441	1446	1455	rBV	210411	273006	18.32%	2.617%
11	10.681	1455	1460	1474	rBV	596563	826799	55.49%	7.926%
12	10.904	1494	1498	1504	rBV	40268	52382	3.52%	0.502%
13	11.375	1573	1578	1586	rBV	357723	475281	31.90%	4.556%
14	11.892	1662	1666	1679	rBV3	36920	70185	4.71%	0.673%
15	12.386	1745	1750	1754	rBV	14170	19673	1.32%	0.189%
16	12.957	1842	1847	1857	rBV	1171528	1489969	100.00%	14.283%
17	13.257	1895	1898	1902	rVB2	15540	17665	1.19%	0.169%
18	13.427	1923	1927	1934	rVB	63859	79940	5.37%	0.766%
19	13.857	1994	2000	2012	rVB3	33124	86649	5.82%	0.831%
20	14.027	2024	2029	2038	rVB	308463	426896	28.65%	4.092%
21	15.521	2277	2283	2297	rVB	174990	315983	21.21%	3.029%




Sum of corrected areas: 10431953

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140952.D
Acq On : 20 Dec 2024 15:55
Operator : RC/JU
Sample : P5306-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-07-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

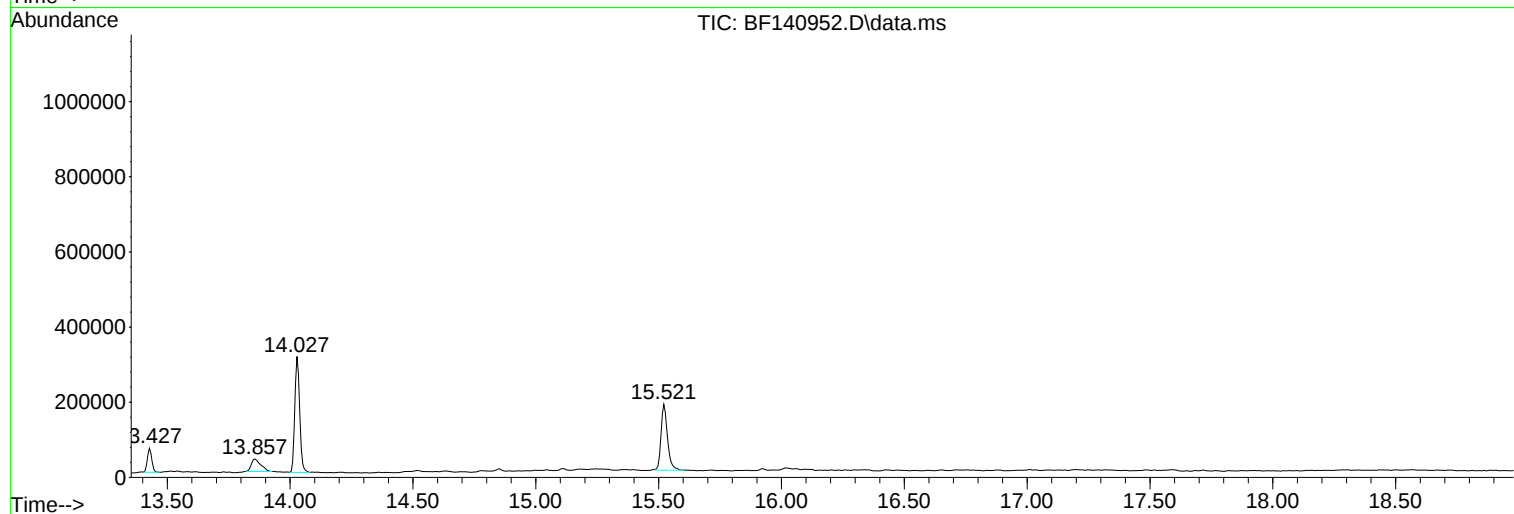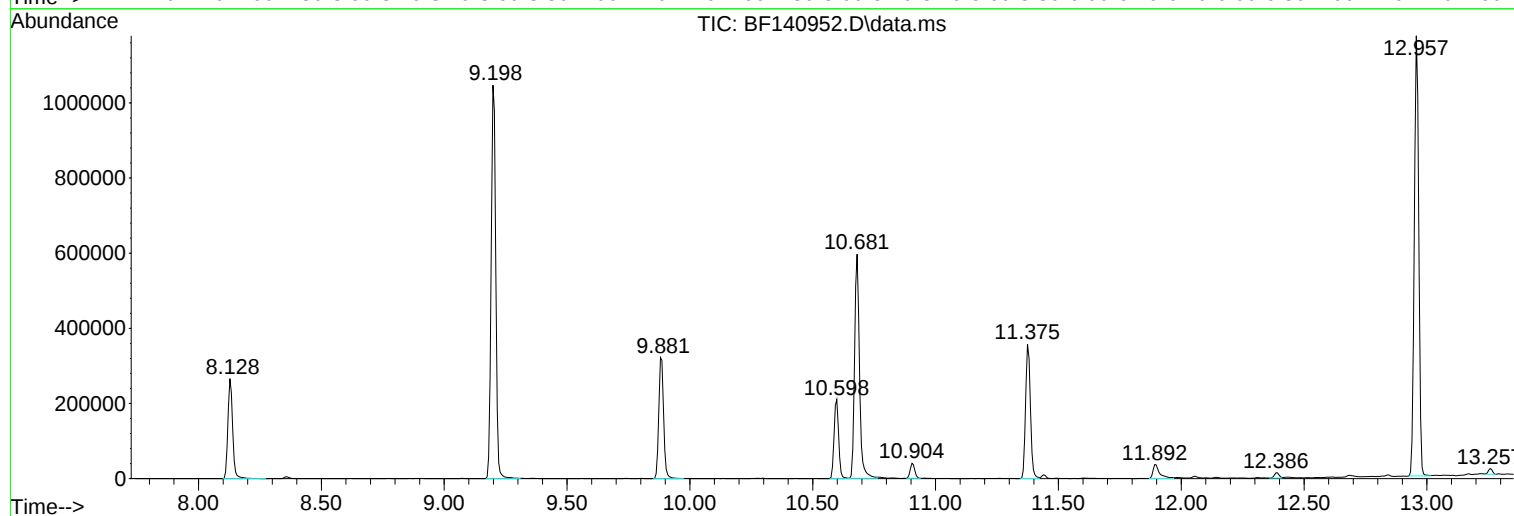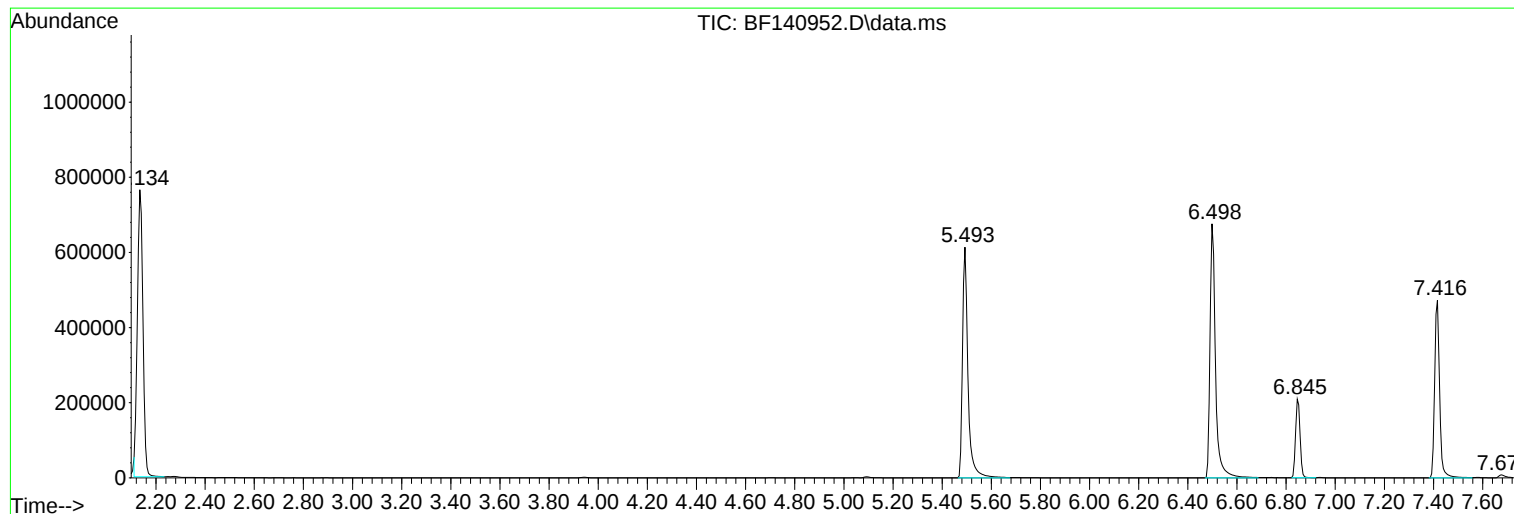

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140952.D
Acq On : 20 Dec 2024 15:55
Operator : RC/JU
Sample : P5306-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-07-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140952.D
Acq On : 20 Dec 2024 15:55
Operator : RC/JU
Sample : P5306-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-07-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------