

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140953.D
 Acq On : 20 Dec 2024 16:21
 Operator : RC/JU
 Sample : P5306-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-08-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	3	12	28	rVB	1114156	1842603	73.12%	10.684%
2	5.498	573	579	606	rBV	1129990	1694685	67.25%	9.826%
3	6.504	744	750	778	rBV	1231734	1836730	72.89%	10.650%
4	6.845	804	808	817	rBV	227172	288997	11.47%	1.676%
5	7.416	899	905	916	rBV	896108	1214202	48.18%	7.040%
6	7.669	944	948	957	rBV	21697	36065	1.43%	0.209%
7	7.781	963	967	977	rVB	19290	27864	1.11%	0.162%
8	8.128	1021	1026	1043	rBV	302770	398430	15.81%	2.310%
9	9.204	1202	1209	1218	rBV	1794028	2407055	95.52%	13.957%
10	9.880	1315	1324	1337	rBV	374997	504603	20.02%	2.926%
11	10.598	1441	1446	1455	rBV	120590	155001	6.15%	0.899%
12	10.680	1455	1460	1473	rBV	1173525	1625971	64.52%	9.428%
13	11.374	1573	1578	1587	rBV	420427	556066	22.07%	3.224%
14	11.598	1611	1616	1623	rBV6	9697	26887	1.07%	0.156%
15	11.898	1661	1667	1678	rBV2	99769	191153	7.59%	1.108%
16	12.139	1700	1708	1713	rBV4	18926	33347	1.32%	0.193%
17	12.680	1796	1800	1808	rBV6	26723	58738	2.33%	0.341%
18	12.821	1820	1824	1825	rBV2	20422	26920	1.07%	0.156%
19	12.963	1842	1848	1853	rBV	1870015	2519989	100.00%	14.611%
20	13.174	1881	1884	1892	rVB2	24817	39542	1.57%	0.229%
21	13.468	1930	1934	1939	rVV	300324	393952	15.63%	2.284%
22	13.516	1939	1942	1949	rVB	29862	41351	1.64%	0.240%
23	13.851	1994	1999	2012	rBV3	57680	135925	5.39%	0.788%
24	14.027	2025	2029	2037	rVB	286968	387759	15.39%	2.248%
25	14.163	2048	2052	2056	rBV	34029	47235	1.87%	0.274%
26	14.480	2101	2106	2111	rBV2	74821	119901	4.76%	0.695%
27	14.780	2153	2157	2161	rBV2	36572	50137	1.99%	0.291%
28	15.521	2275	2283	2296	rVB	200318	396042	15.72%	2.296%
29	15.927	2348	2352	2357	rVB	26955	43143	1.71%	0.250%
30	16.433	2434	2438	2449	rVB3	25330	59064	2.34%	0.342%
31	17.021	2534	2538	2548	rVB3	20357	45770	1.82%	0.265%
32	17.721	2653	2657	2666	rVB5	16983	41494	1.65%	0.241%




Sum of corrected areas: 17246621

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140953.D
Acq On : 20 Dec 2024 16:21
Operator : RC/JU
Sample : P5306-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-08-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

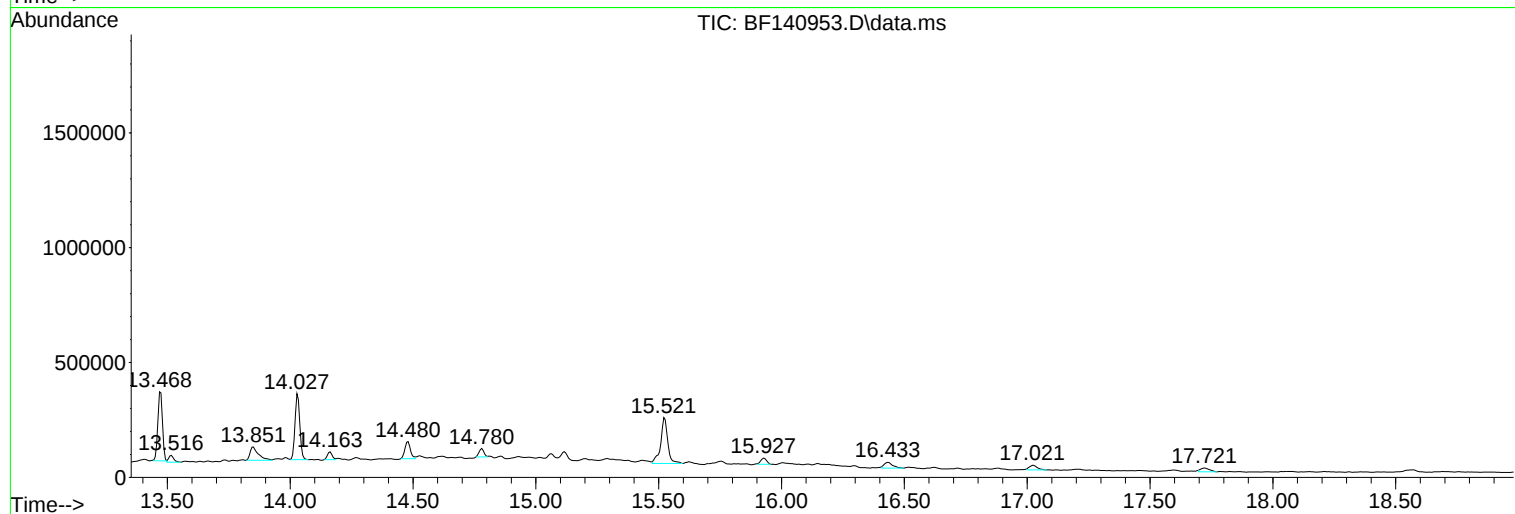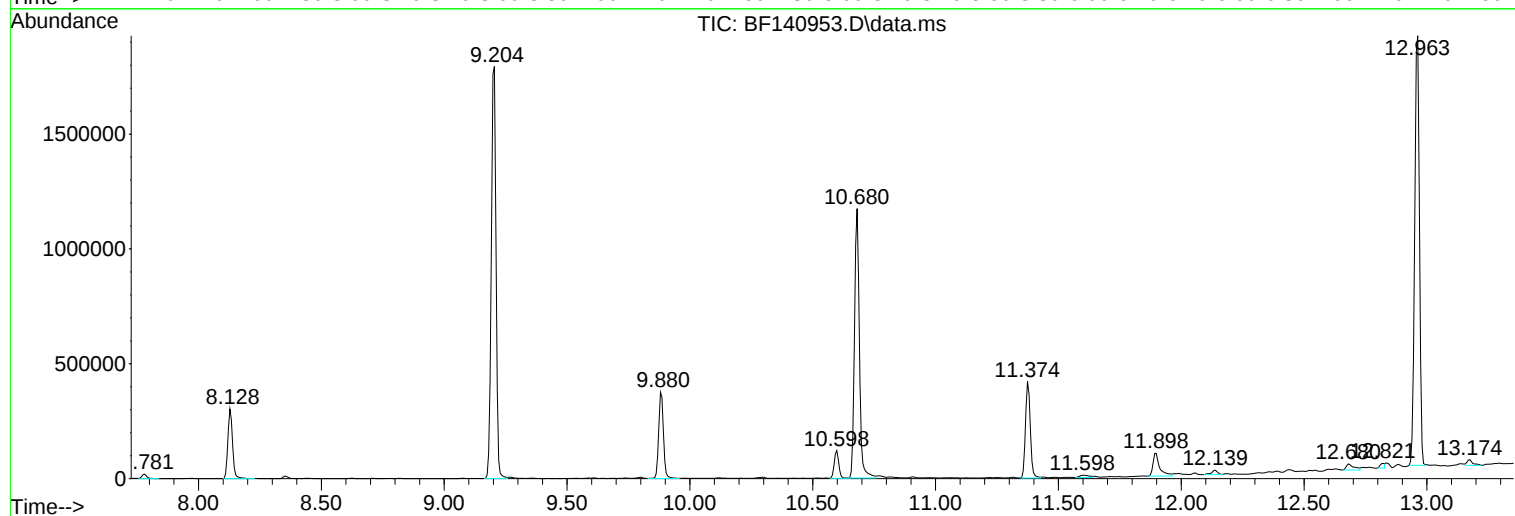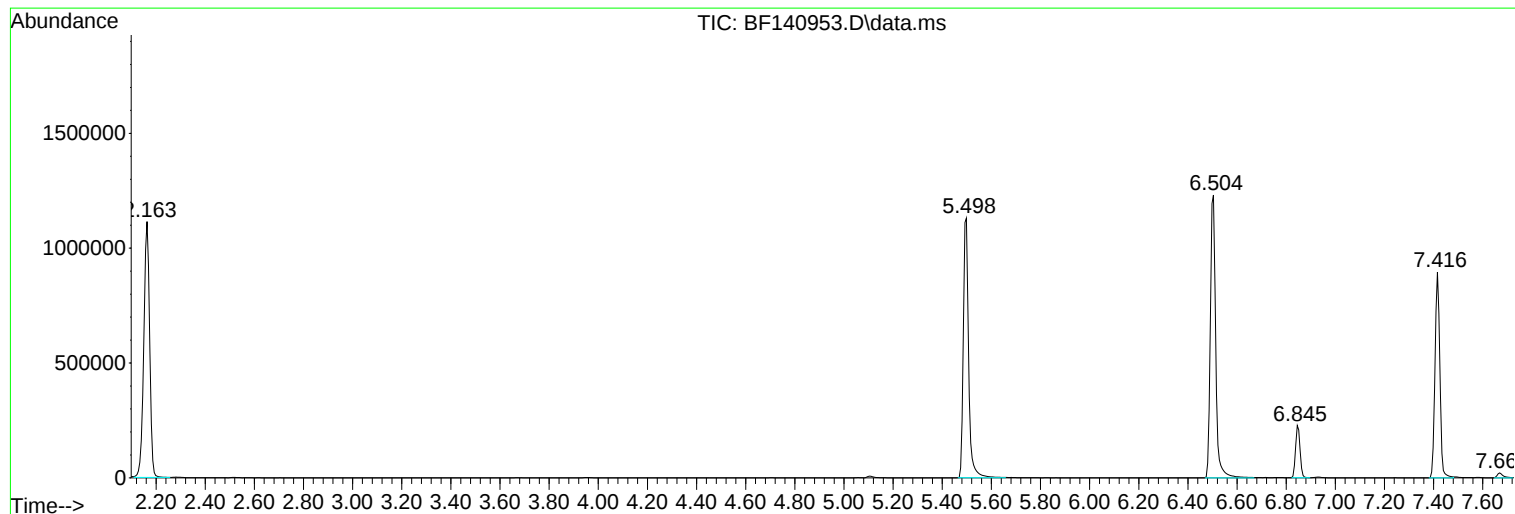

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140953.D
Acq On : 20 Dec 2024 16:21
Operator : RC/JU
Sample : P5306-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-08-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140953.D
Acq On : 20 Dec 2024 16:21
Operator : RC/JU
Sample : P5306-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-08-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------