

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140954.D
 Acq On : 20 Dec 2024 16:48
 Operator : RC/JU
 Sample : P5306-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-09-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	3	12	28	rVB	1188747	2016700	84.97%	12.904%
2	5.498	573	579	604	rBV	1154309	1715990	72.30%	10.980%
3	6.504	744	750	777	rBV	1232109	1832880	77.22%	11.727%
4	6.845	804	808	816	rBV	212057	273936	11.54%	1.753%
5	7.416	899	905	930	rBV	862297	1191206	50.19%	7.622%
6	7.669	944	948	960	rBV	18443	33331	1.40%	0.213%
7	8.128	1021	1026	1048	rBV	277048	369226	15.56%	2.362%
8	9.204	1202	1209	1219	rBV	1755785	2350614	99.03%	15.040%
9	9.880	1319	1324	1336	rBV	327603	443386	18.68%	2.837%
10	10.598	1441	1446	1455	rBV	107958	135069	5.69%	0.864%
11	10.680	1455	1460	1481	rBV	1105011	1513043	63.75%	9.681%
12	11.374	1573	1578	1586	rBV	369478	484423	20.41%	3.100%
13	11.439	1586	1589	1595	rVB	20799	24697	1.04%	0.158%
14	11.892	1662	1666	1680	rBV3	34379	67991	2.86%	0.435%
15	12.957	1841	1847	1853	rBV	1781133	2373522	100.00%	15.187%
16	13.851	1994	1999	2013	rBV3	34671	92091	3.88%	0.589%
17	14.027	2024	2029	2040	rBV	294429	408605	17.22%	2.614%
18	15.521	2278	2283	2297	rVB	165560	302291	12.74%	1.934%




Sum of corrected areas: 15629001

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140954.D
Acq On : 20 Dec 2024 16:48
Operator : RC/JU
Sample : P5306-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-09-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

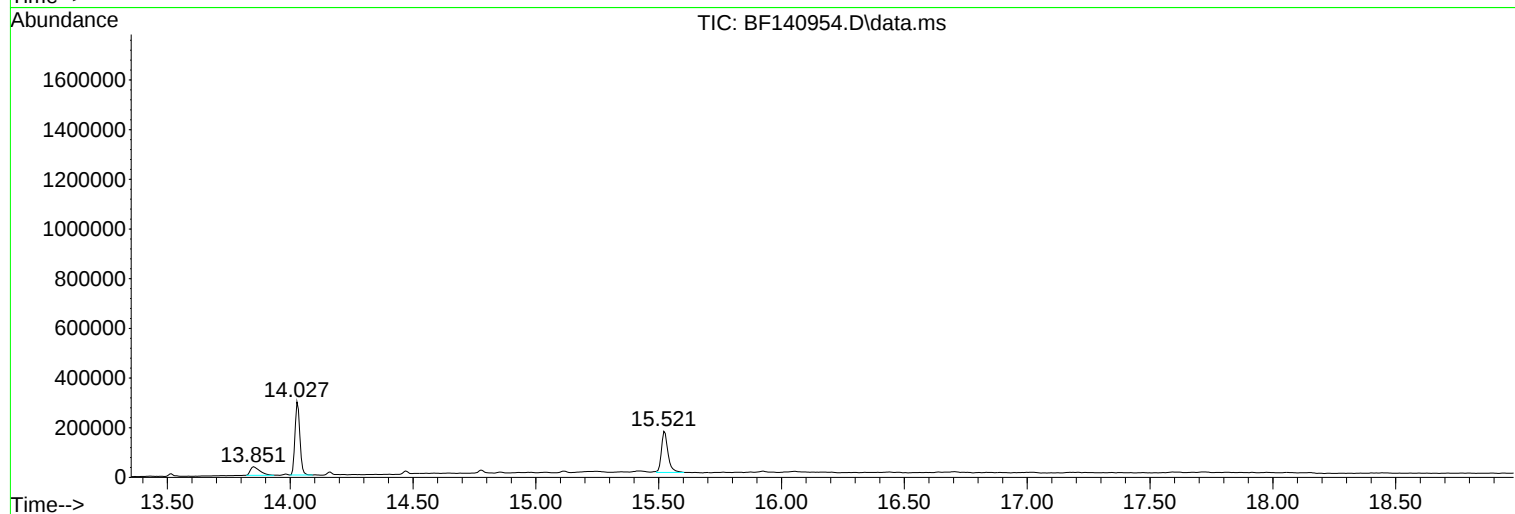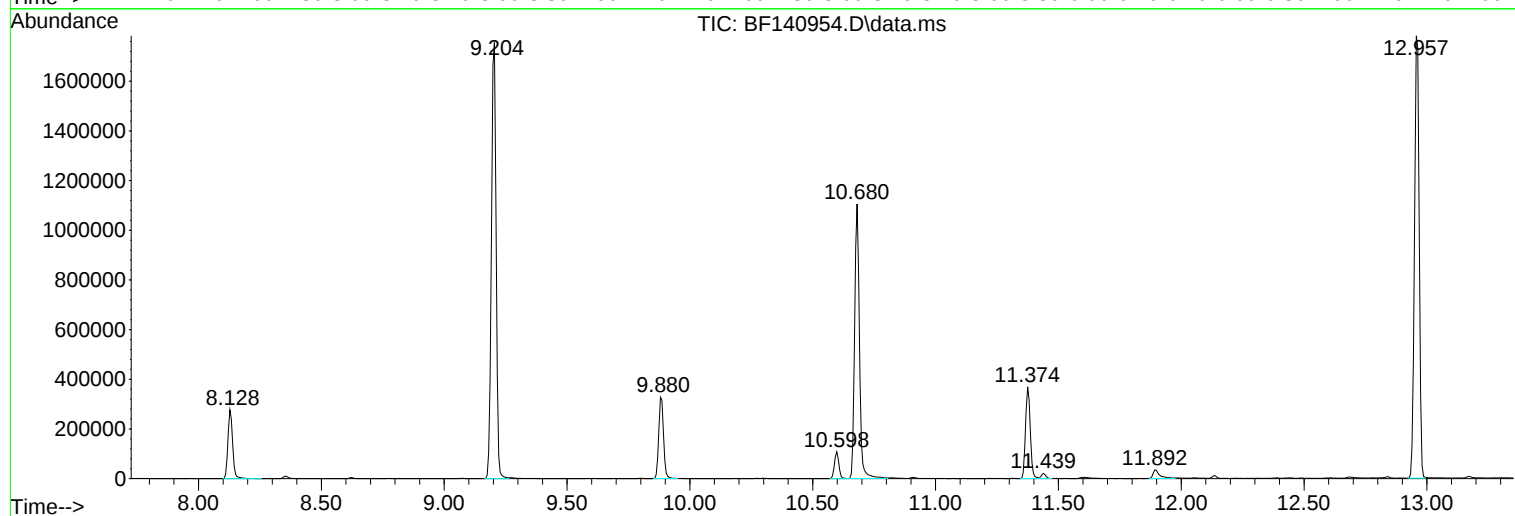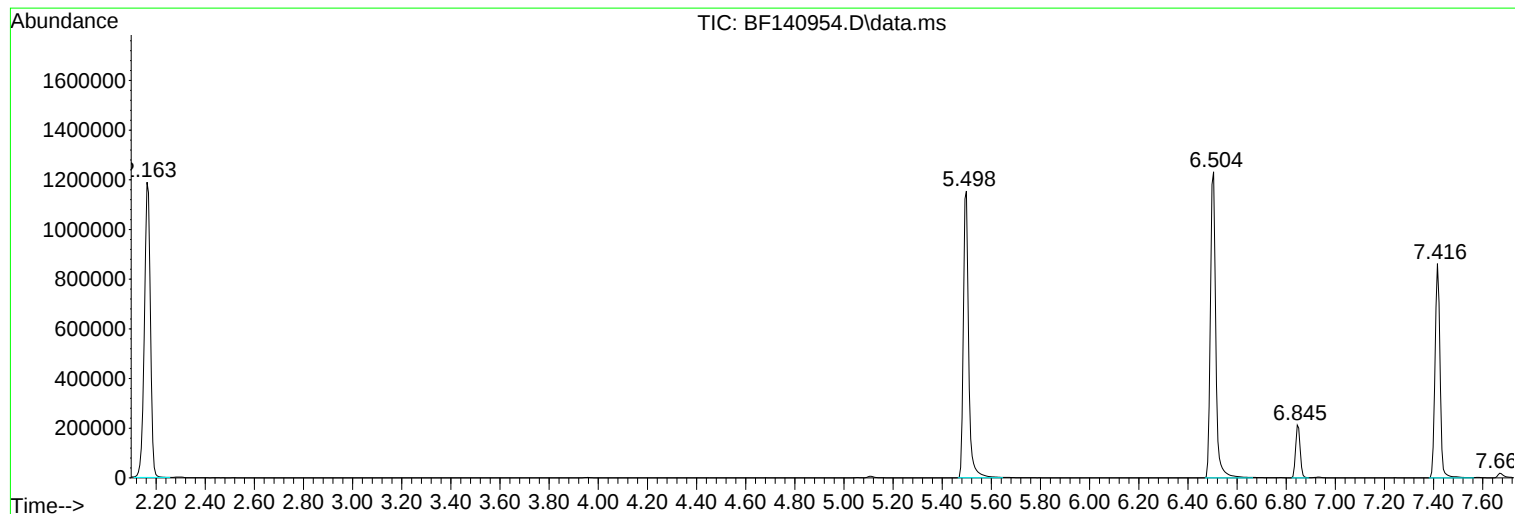

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140954.D
Acq On : 20 Dec 2024 16:48
Operator : RC/JU
Sample : P5306-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-09-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140954.D
Acq On : 20 Dec 2024 16:48
Operator : RC/JU
Sample : P5306-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-09-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------