

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
 Data File : BF140955.D
 Acq On : 20 Dec 2024 17:14
 Operator : RC/JU
 Sample : P5306-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-10-121224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	3	12	28	rVB	1161227	1994830	75.71%	12.732%
2	5.493	573	578	604	rBV	1089322	1645057	62.43%	10.499%
3	6.498	744	749	777	rBV	1201447	1785479	67.76%	11.396%
4	6.846	803	808	817	rBV	220367	279842	10.62%	1.786%
5	7.416	899	905	926	rBV	832807	1153146	43.76%	7.360%
6	8.128	1021	1026	1047	rBV	284593	378648	14.37%	2.417%
7	9.204	1202	1209	1232	rBV	1749522	2377408	90.23%	15.174%
8	9.881	1319	1324	1335	rBV	331005	444762	16.88%	2.839%
9	10.598	1440	1446	1454	rBV	72789	93224	3.54%	0.595%
10	10.681	1454	1460	1483	rVV	1033128	1405952	53.36%	8.973%
11	11.375	1573	1578	1585	rBV	370342	485866	18.44%	3.101%
12	11.598	1610	1616	1634	rBV5	12348	39486	1.50%	0.252%
13	11.892	1661	1666	1678	rBV2	19681	40204	1.53%	0.257%
14	12.133	1702	1707	1712	rBV	37781	46589	1.77%	0.297%
15	12.957	1841	1847	1853	rBV	1973973	2634904	100.00%	16.817%
16	13.851	1993	1999	2016	rBV3	40413	119899	4.55%	0.765%
17	14.027	2024	2029	2040	rVB	300600	412263	15.65%	2.631%
18	15.516	2277	2282	2299	rVB	175562	330566	12.55%	2.110%




Sum of corrected areas: 15668125

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140955.D
Acq On : 20 Dec 2024 17:14
Operator : RC/JU
Sample : P5306-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-10-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

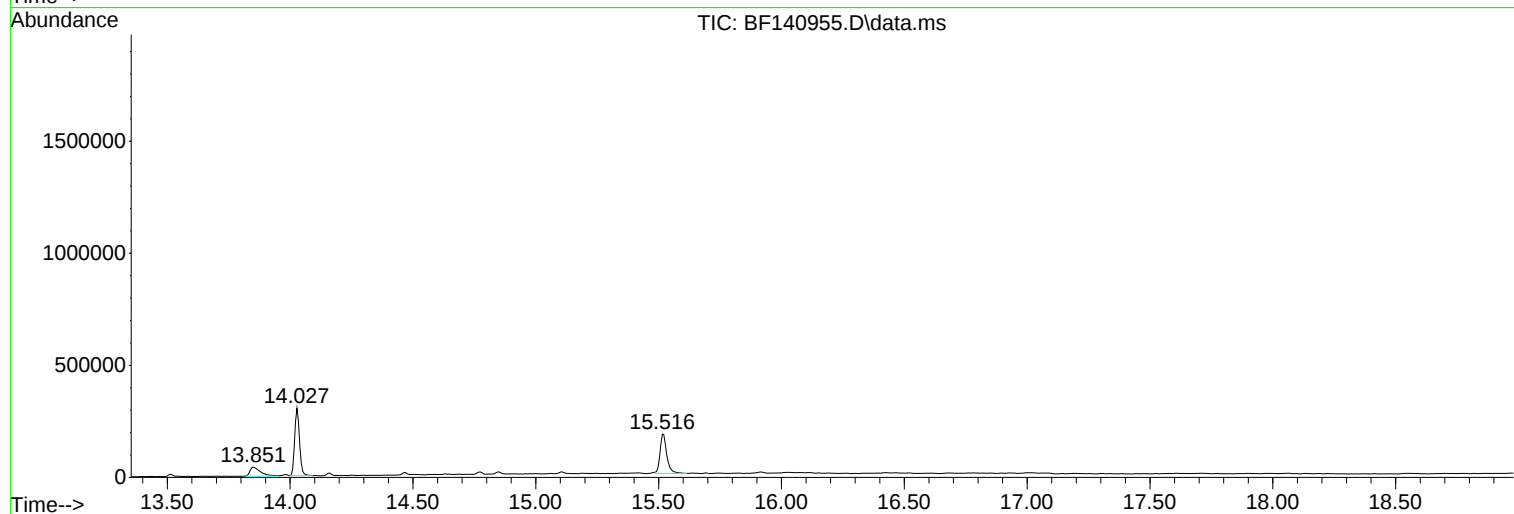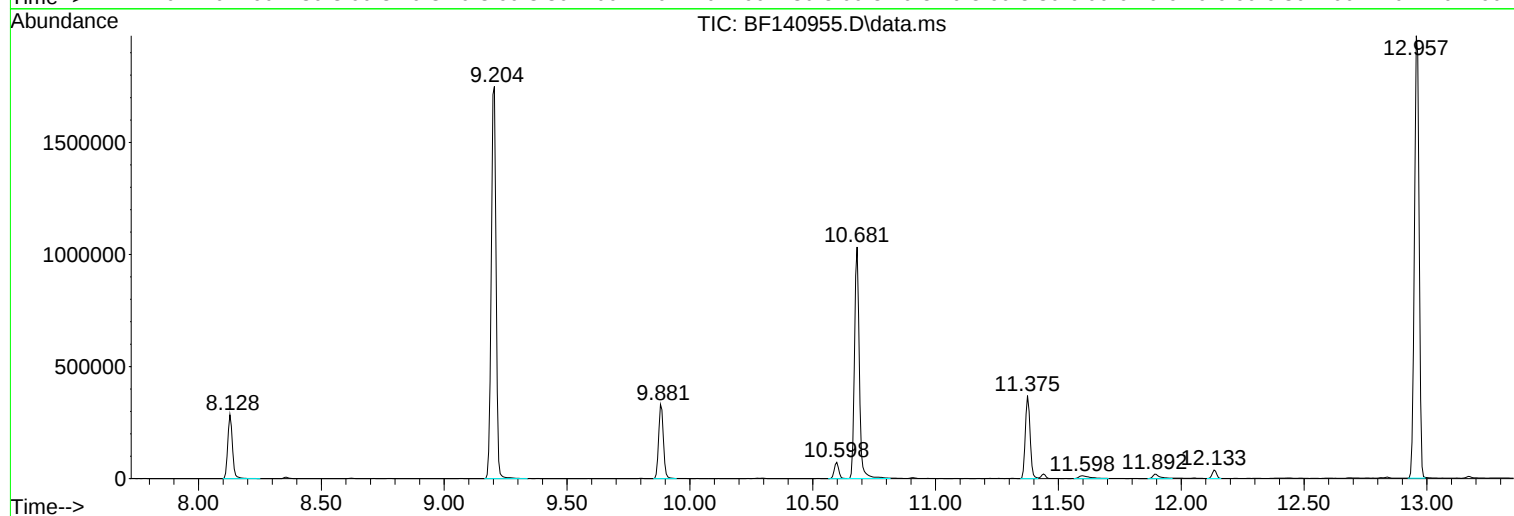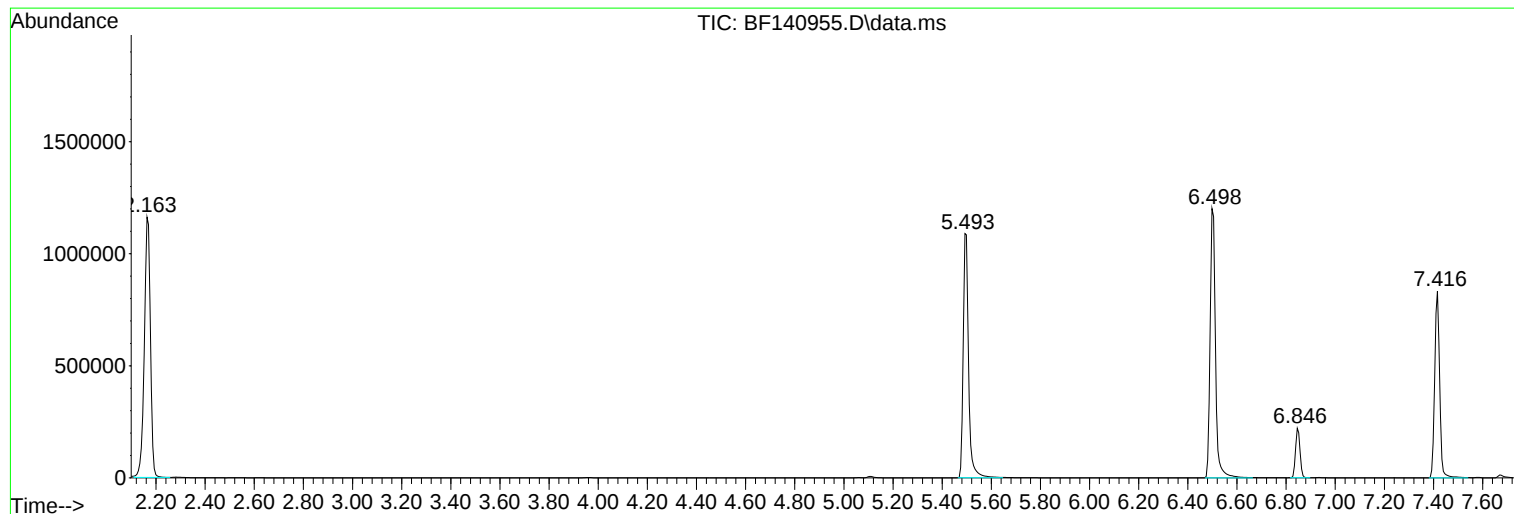

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140955.D
Acq On : 20 Dec 2024 17:14
Operator : RC/JU
Sample : P5306-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-10-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140955.D
Acq On : 20 Dec 2024 17:14
Operator : RC/JU
Sample : P5306-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-10-121224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------