


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140941.D
Acq On : 20 Dec 2024 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 16 16:59:50 2024

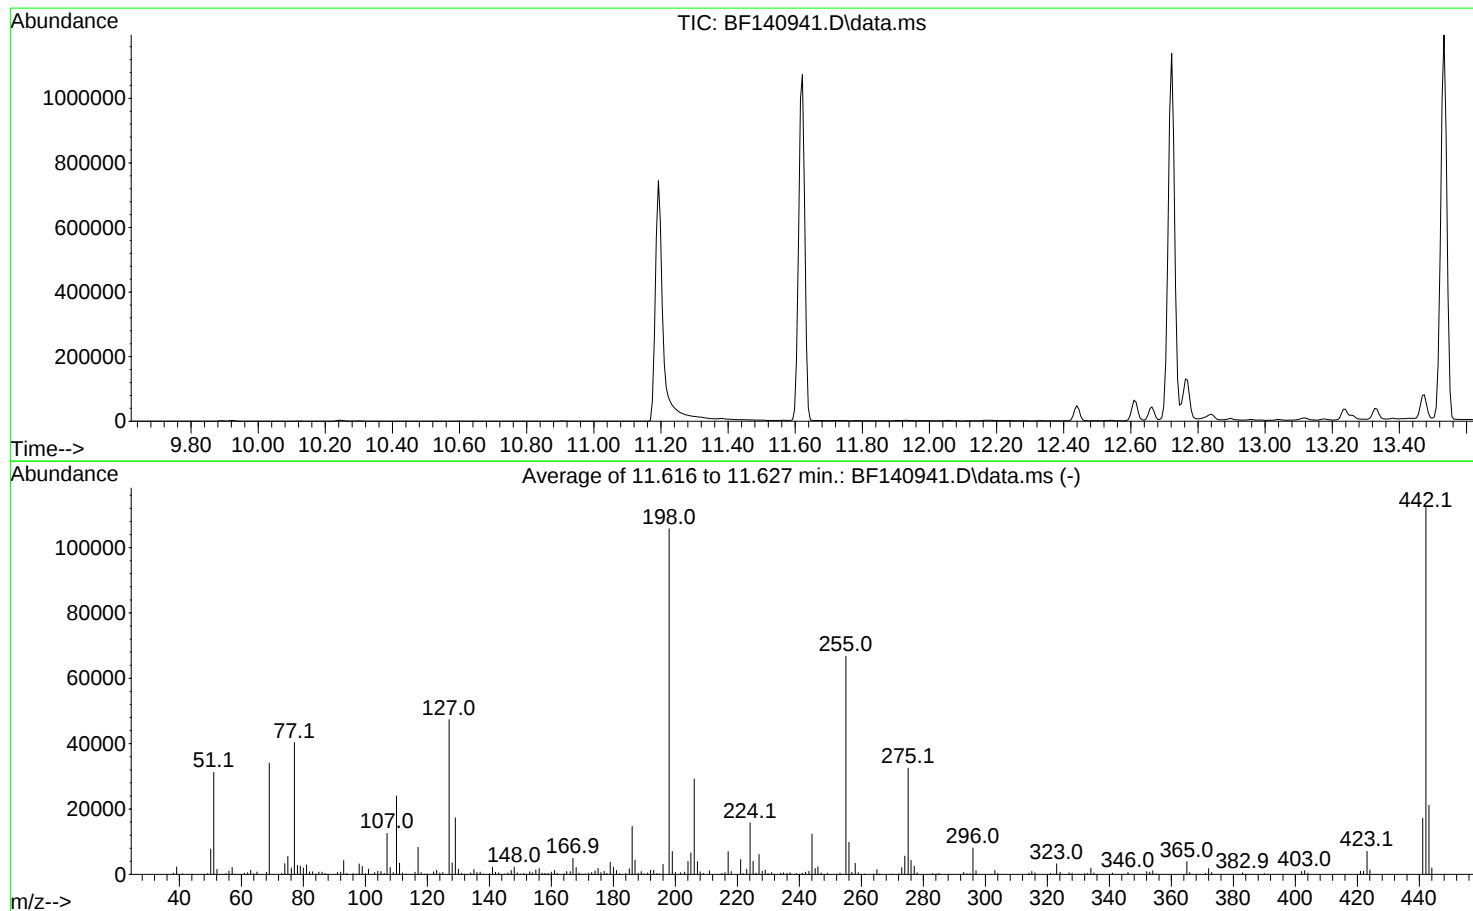

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	31259	PASS
68	69	0.00	2	1.9	646	PASS
69	198	0.00	100	32.2	34051	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	47344	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105763	PASS
199	198	5	9	6.6	7029	PASS
275	198	10	60	30.8	32541	PASS
365	198	1	100	3.7	3936	PASS
441	198	0.01	100	16.2	17150	PASS
442	442	50	100	100.0	112581	PASS
443	442	15	24	18.7	21093	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/20/2024	BNA_F	<u>BF1408941.D</u>
Compound Name	Response	Retention Time
DDT	616229	13.533
DDD	15993	13.239
DDE	2518	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18511	634740	2.92

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140941.D
Acq On : 20 Dec 2024 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 11:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

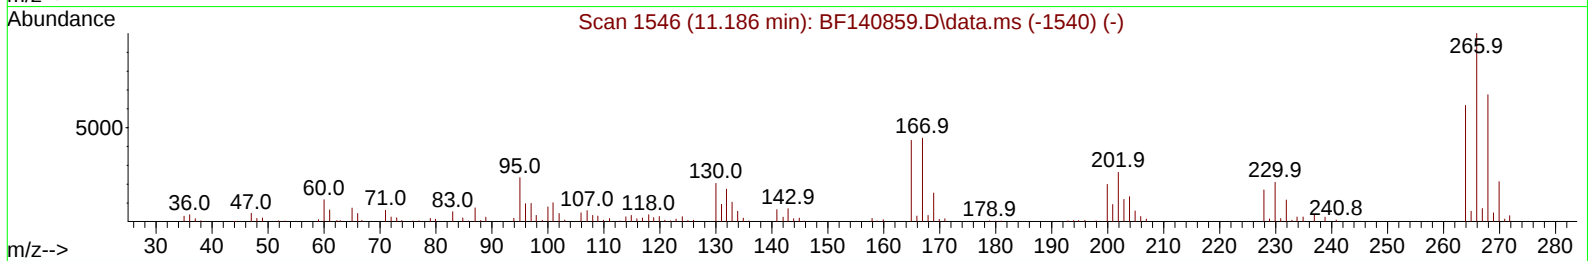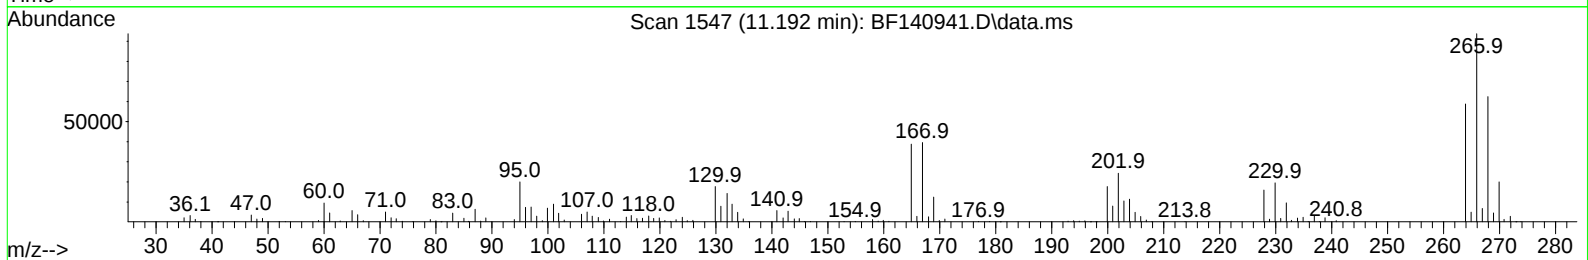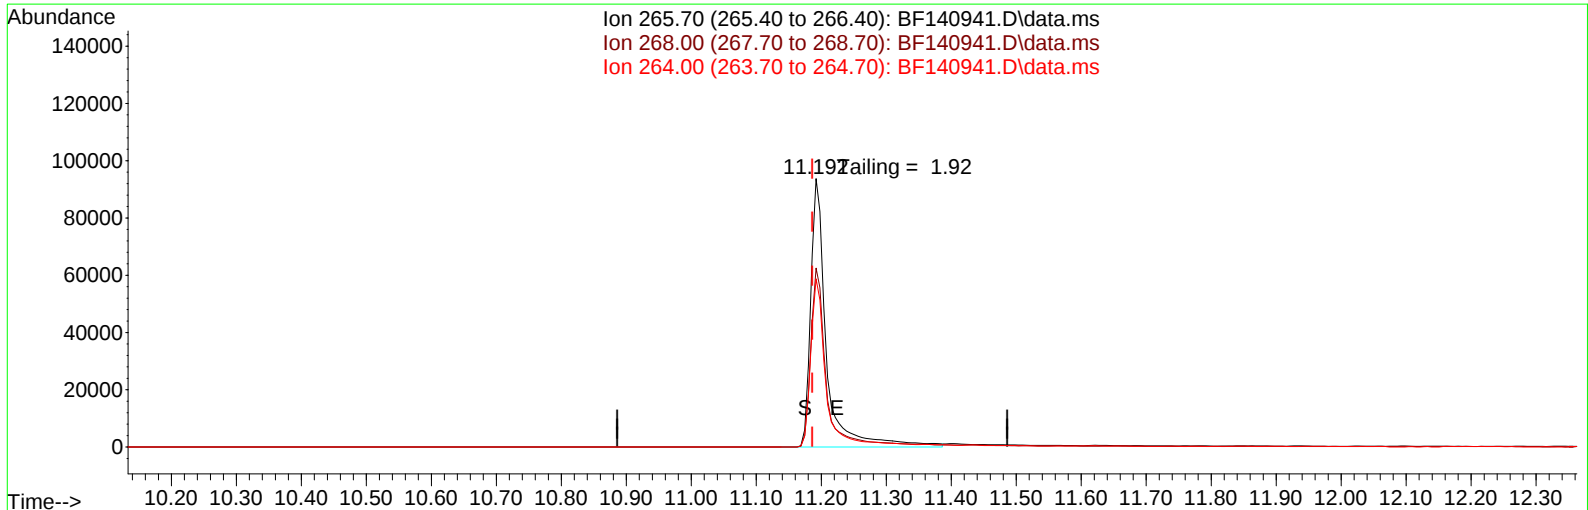

TIC: BF140941.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.006) 18269.88 ng




response 157756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	66.64
264.00	61.80	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122024\
Data File : BF140941.D
Acq On : 20 Dec 2024 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 11:56:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

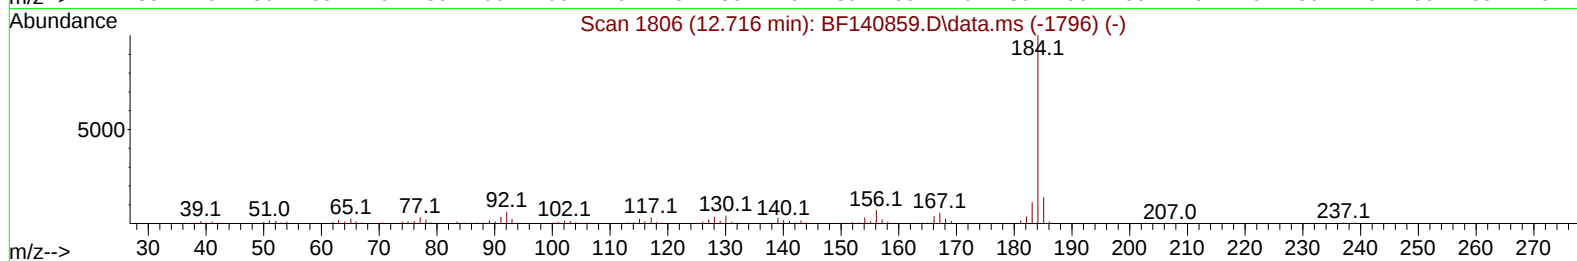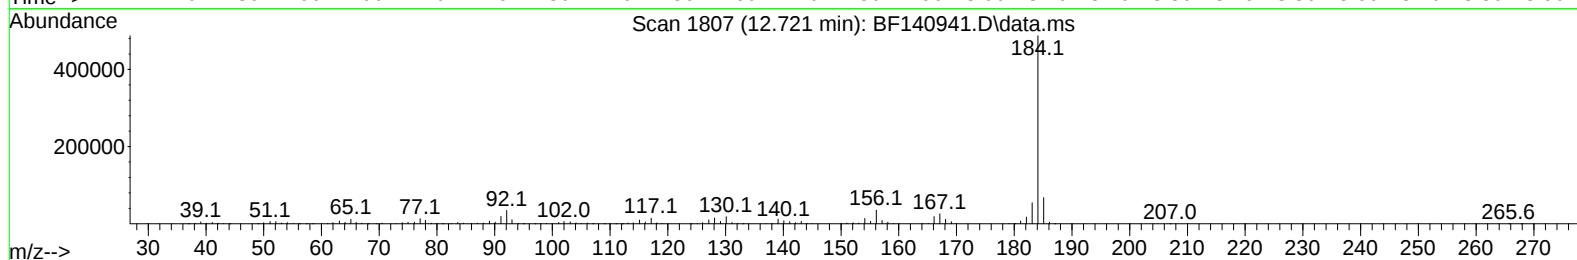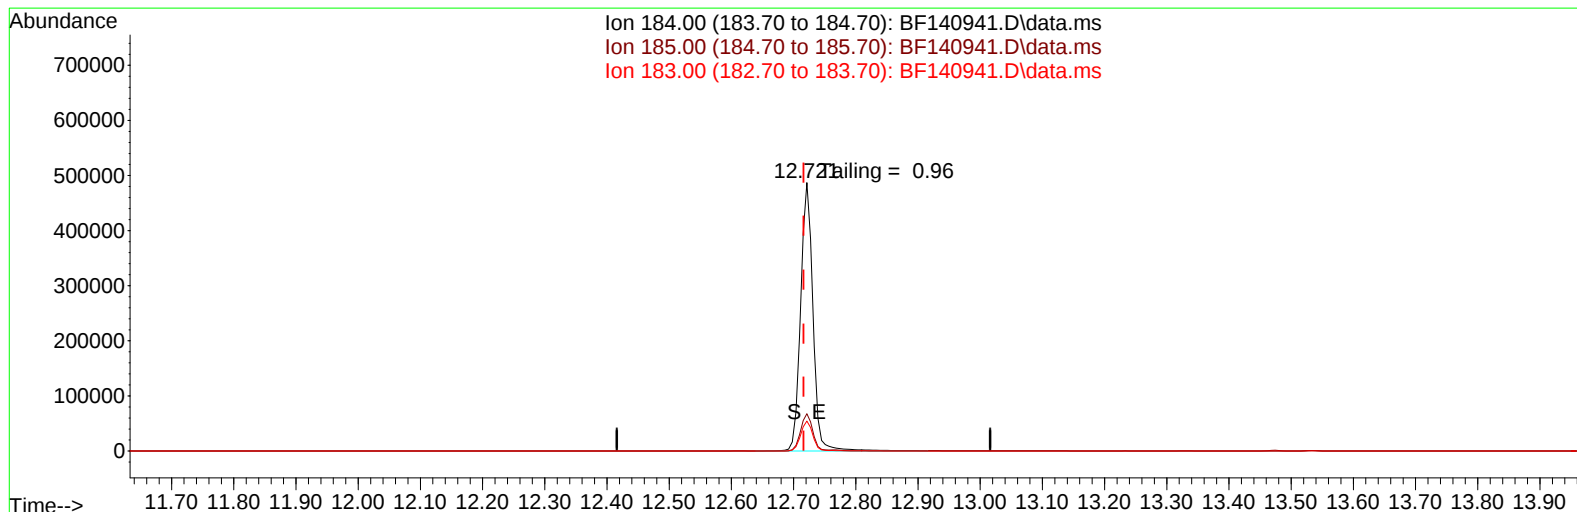

TIC: BF140941.D\data.ms

(77) Benzidine

12.721min (+ 0.005) 28215.57 ng

response 676070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.93
183.00	11.20	11.19
0.00	0.00	0.00