
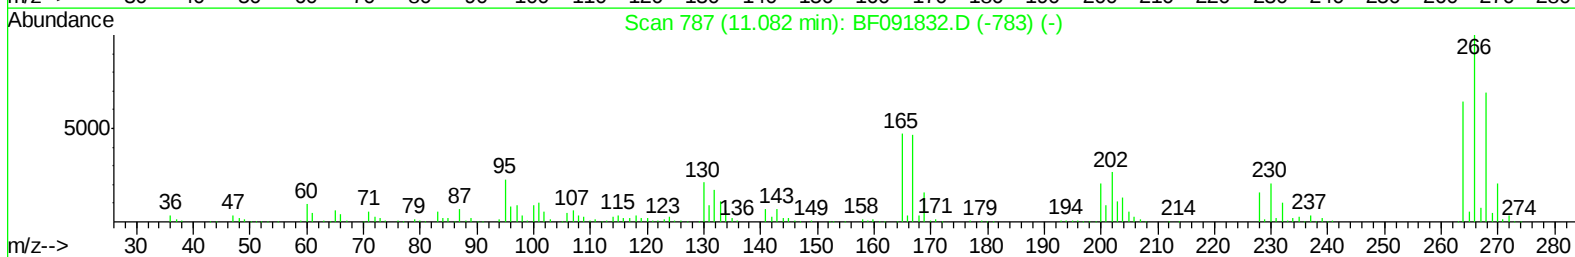
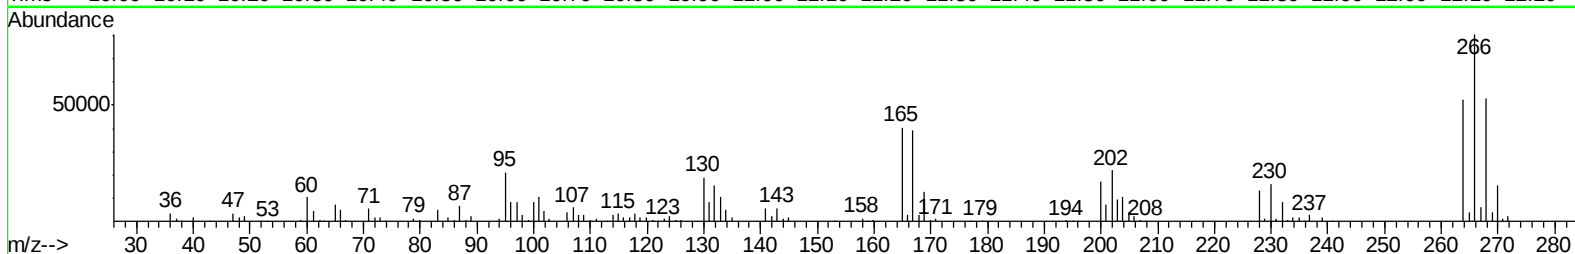


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122116\
Data File : BF091848.D
Acq On : 21 Dec 2016 22:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 07:47:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

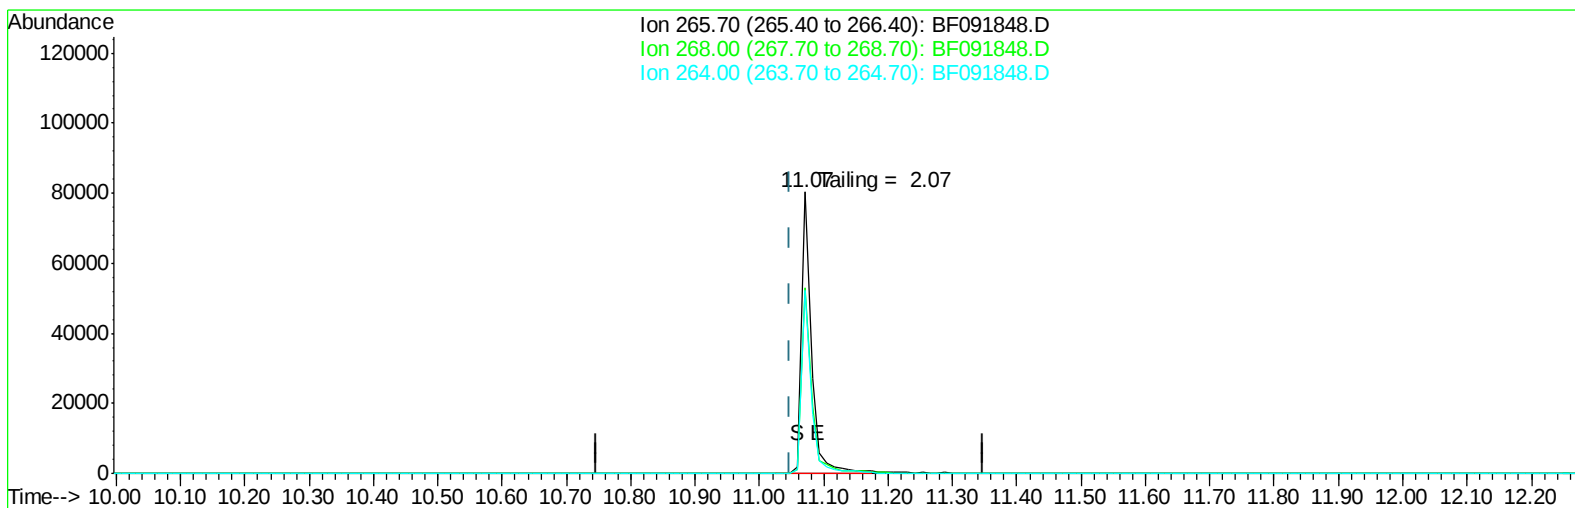

TIC: BF091848.D

(69) Pentachlorophenol (C)




11.071min (+0.023) 56911.52ng

response 86939

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.87
264.00	62.90	64.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF122116\
Data File : BF091848.D
Acq On : 21 Dec 2016 22:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 07:47:22 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

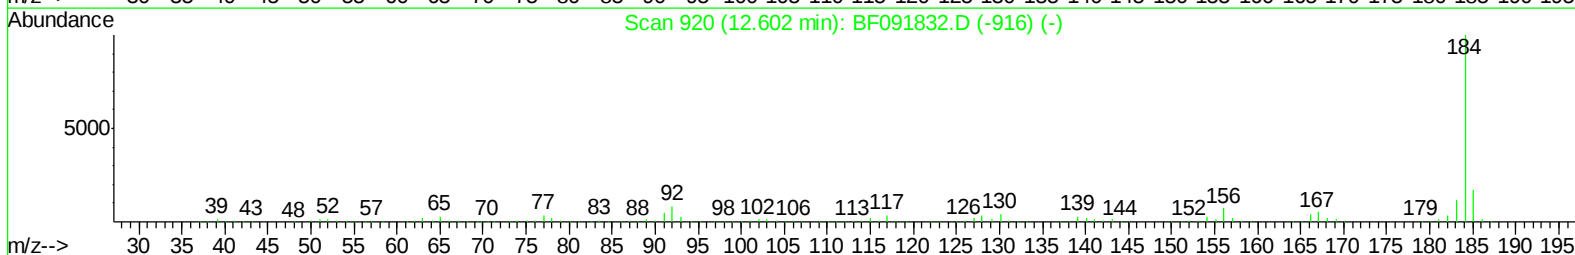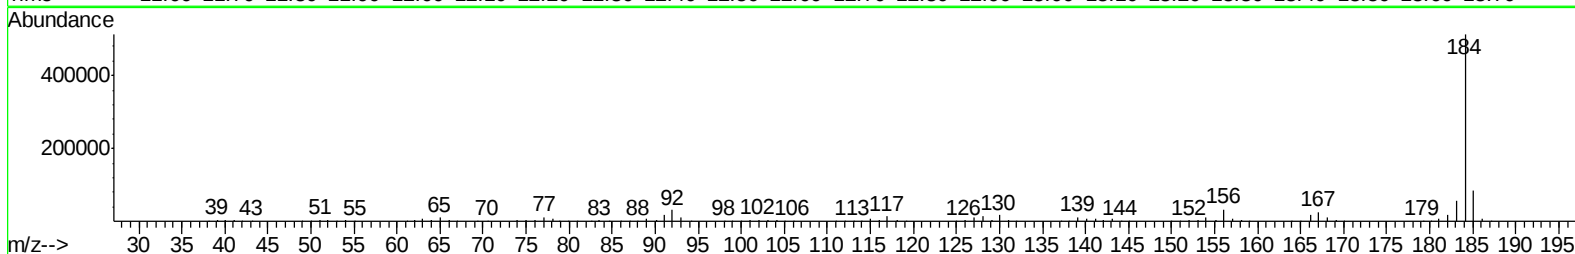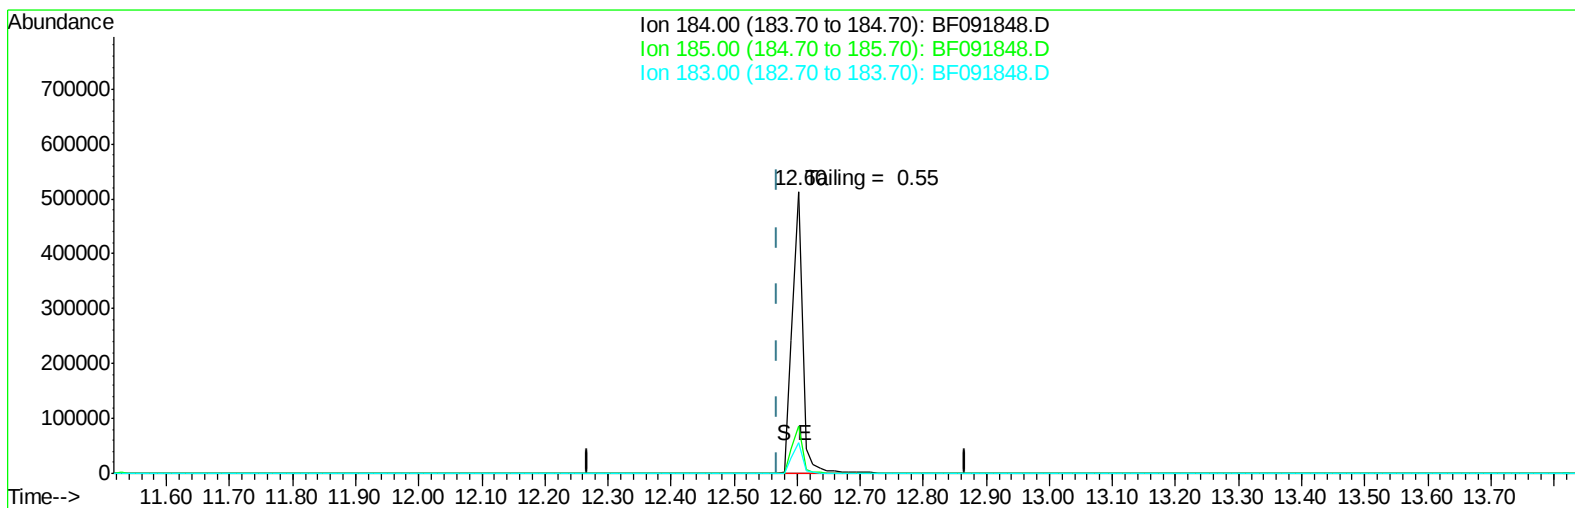

TIC: BF091848.D

(76) Benzidine

12.602min (+0.034) -20.00ng

response 585553

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.70
183.00	11.50	10.83
0.00	0.00	0.00