

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122116\
 Data File : BF091870.D
 Acq On : 22 Dec 2016 8:01
 Operator : UM/SJ
 Sample : H6156-16
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-12A

Quant Time: Dec 22 16:08:34 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 16:17:51 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	306381	20.00	ng	0.00
21) Naphthalene-d8	8.03	136	1264795	20.00	ng	-0.01
38) Acenaphthene-d10	9.78	164	632268	20.00	ng	-0.01
63) Phenanthrene-d10	11.26	188	1082688	20.00	ng	0.00
75) Chrysene-d12	13.89	240	759805	20.00	ng	-0.01
86) Perylene-d12	15.29	264	673597	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	1159713	63.20	ng	0.01
7) Phenol-d6	6.40	99	936716	41.81	ng	-0.01
23) Nitrobenzene-d5	7.31	82	2054971	90.35	ng	-0.01
41) 2,4,6-Tribromophenol	10.58	330	744083	142.20	ng	0.00
44) 2-Fluorobiphenyl	9.12	172	3265050	109.53	ng	0.00
78) Terphenyl-d14	12.85	244	2209584	70.53	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122116\
Data File : BF091870.D
Acq On : 22 Dec 2016 8:01
Operator : UM/SJ
Sample : H6156-16
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-12A

Quant Time: Dec 22 16:08:34 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 16:17:51 2016
Response via : Initial Calibration

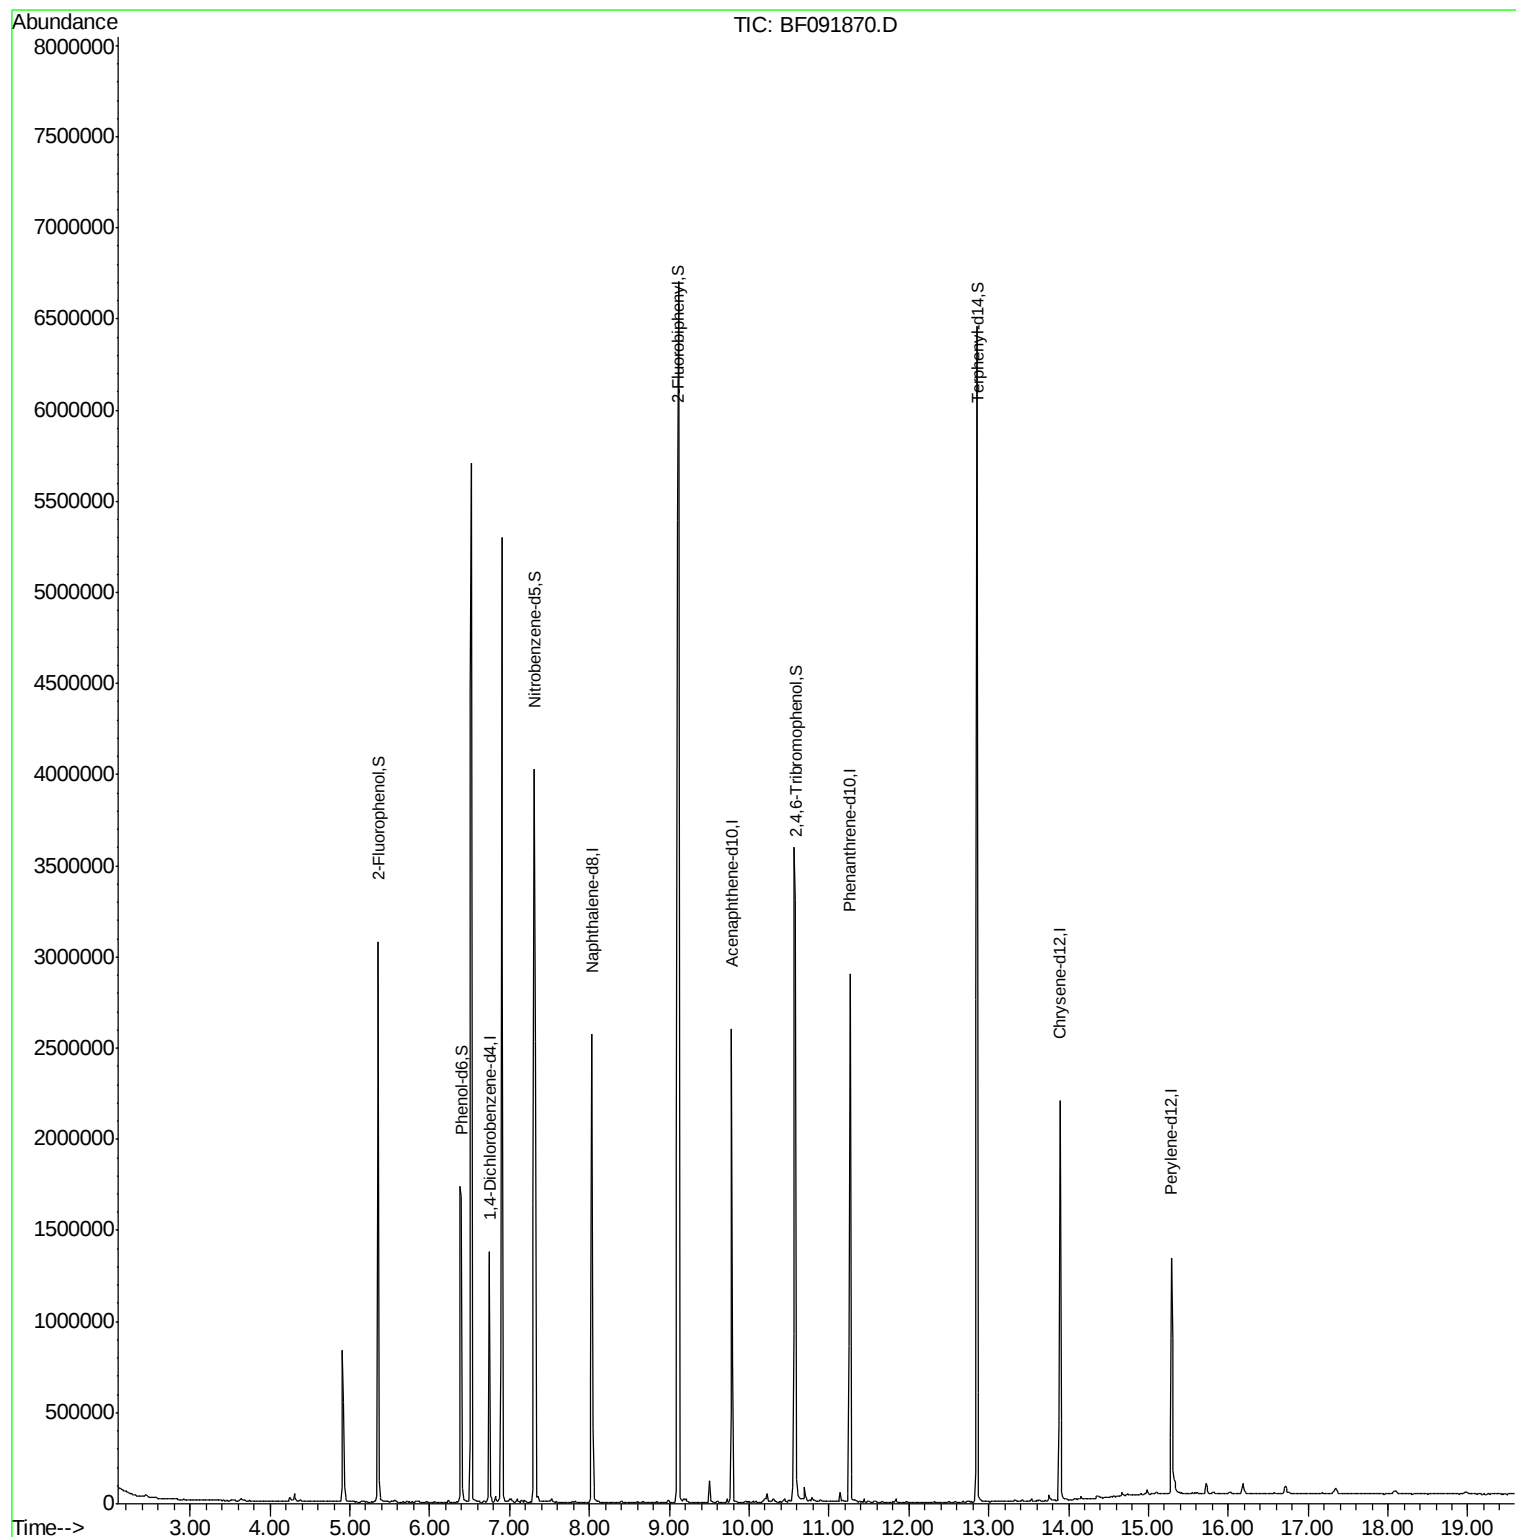

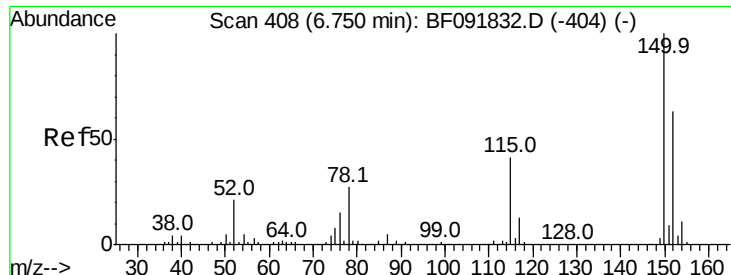

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.75 min Scan# 408

Delta R.T. -0.00 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01

Instrument :

BNA_F

ClientSampleId :

MW-12A


Tot Ion:152 Resp: 306381

Ion Ratio Lower Upper

152 100

150 153.9 124.9 187.3




115 51.6 46.0 69.0

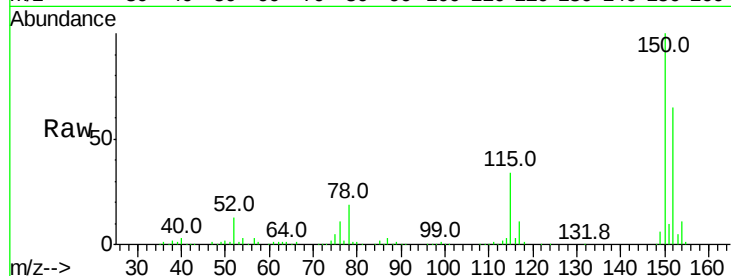

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

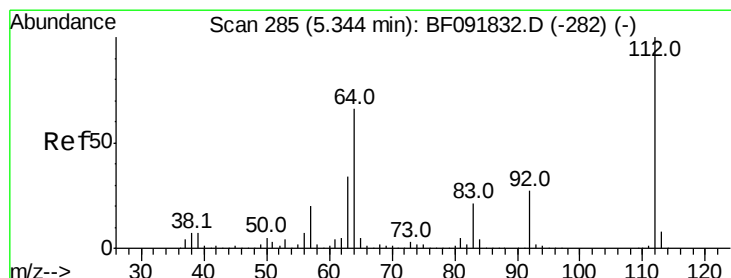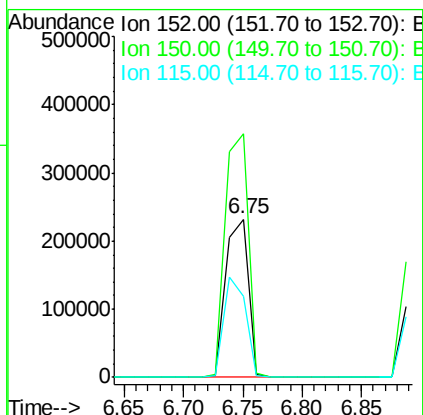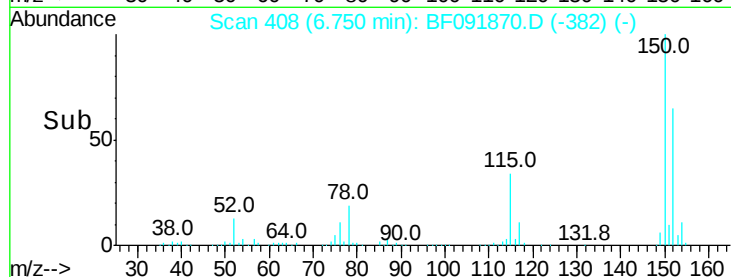

#5

2-Fluorophenol

Concen: 63.20 ng

RT: 5.36 min Scan# 286

Delta R.T. 0.01 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01


Tgt Ion:112 Resp: 1159713

Ion Ratio Lower Upper

112 100

64 52.2 46.1 69.1



63 25.5 23.8 35.6

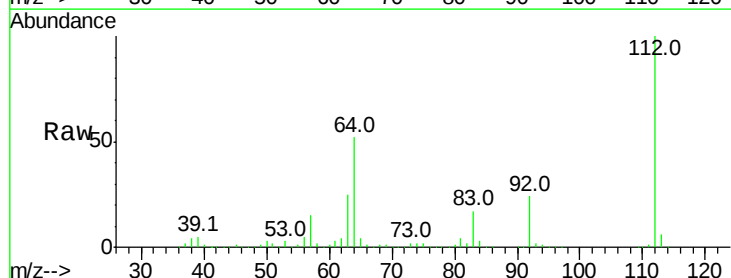


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

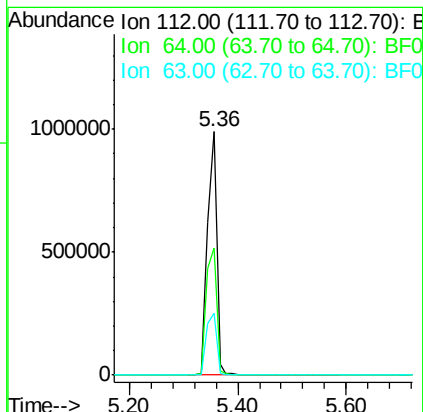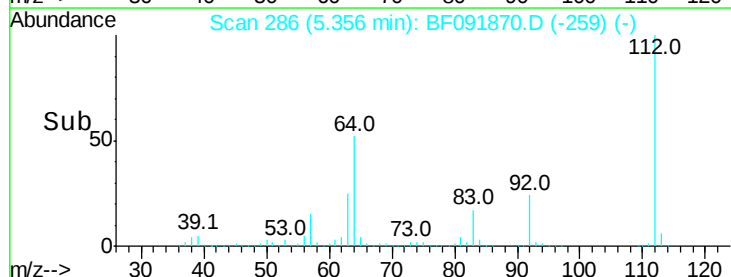

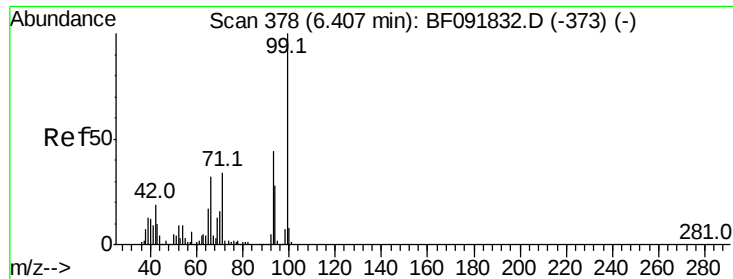

#7

Phenol-d6

Concen: 41.81 ng

RT: 6.40 min Scan# 377

Delta R.T. -0.01 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01

Instrument :

BNA_F

ClientSampleId :

MW-12A





Tot Ion: 99 Resp: 936716

Ion Ratio Lower Upper

99 100

42 12.5 15.6 23.4#

71 25.2 27.5 41.3#

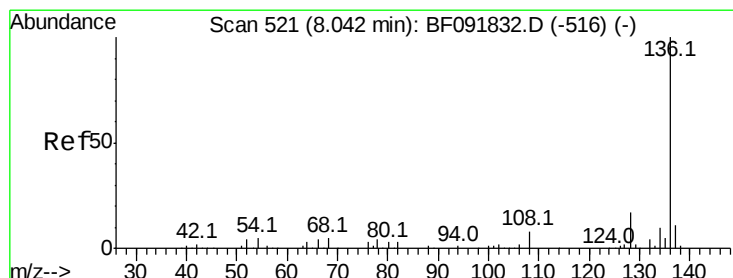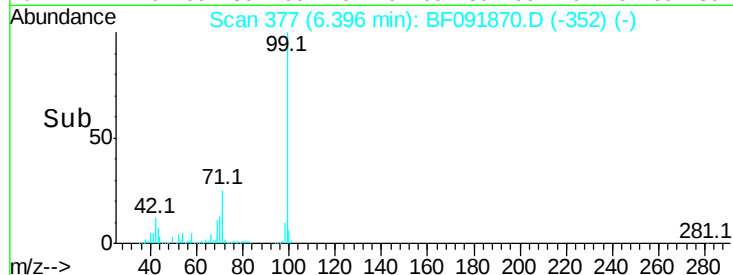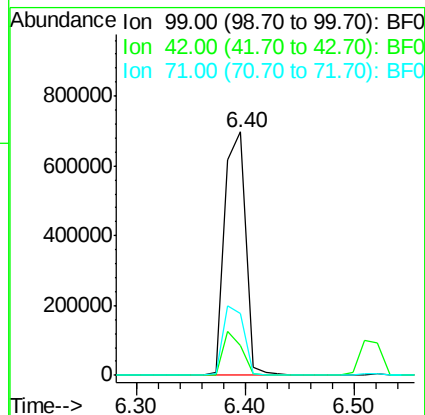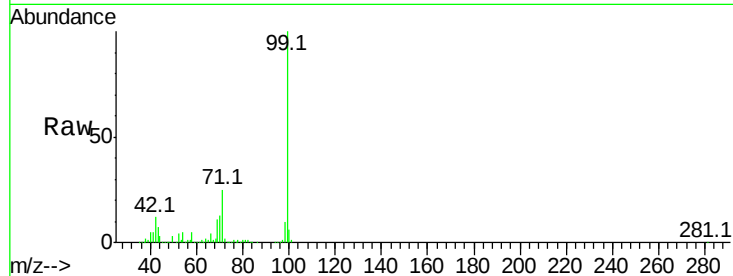

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.03 min Scan# 520

Delta R.T. -0.01 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01

Tgt Ion: 136 Resp: 1264795




Ion Ratio Lower Upper


136 100

137 11.4 8.4 12.6

54 8.6 4.5 6.7#

68 7.5 3.6 5.4#

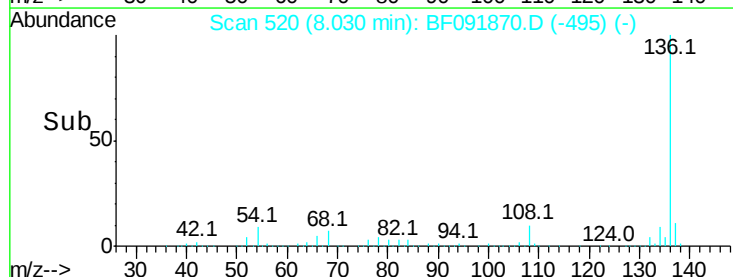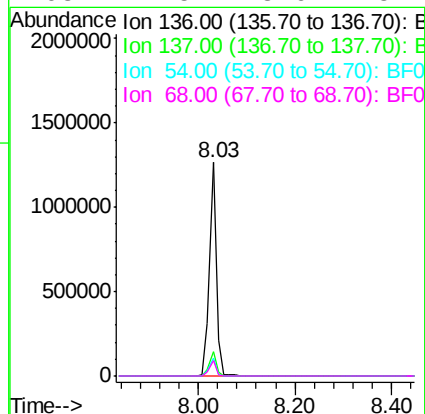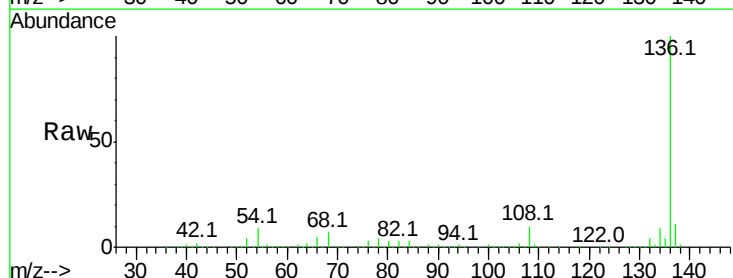

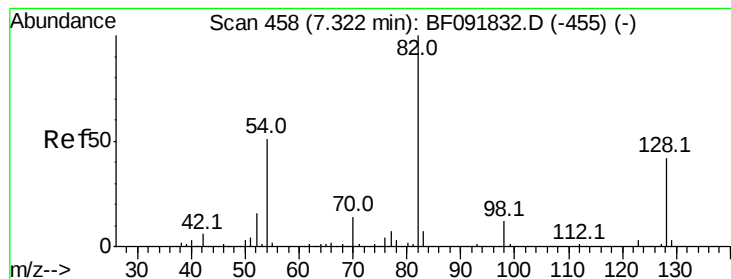

#23

Nitrobenzene-d5

Concen: 90.35 ng

RT: 7.31 min Scan# 457

Delta R.T. -0.01 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01

Instrument :

BNA_F

ClientSampleId :

MW-12A


Tot Ion: 82 Resp: 2054971

Ion Ratio Lower Upper

82 100

128 41.8 34.6 52.0




54 49.3 39.5 59.3

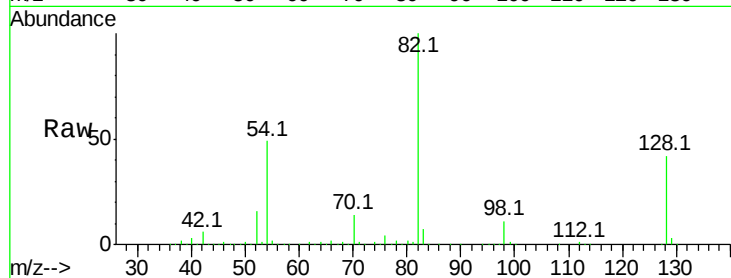

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

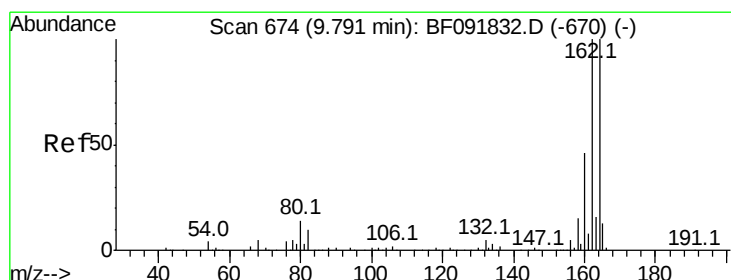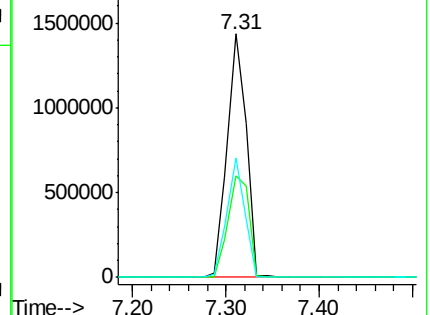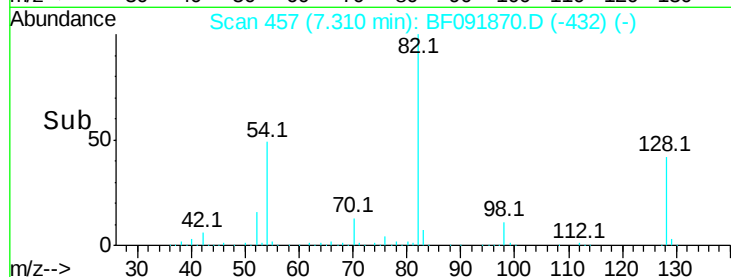

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.78 min Scan# 673

Delta R.T. -0.01 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01


Tgt Ion:164 Resp: 632268

Ion Ratio Lower Upper

164 100

162 101.1 80.2 120.2



160 45.2 36.9 55.3

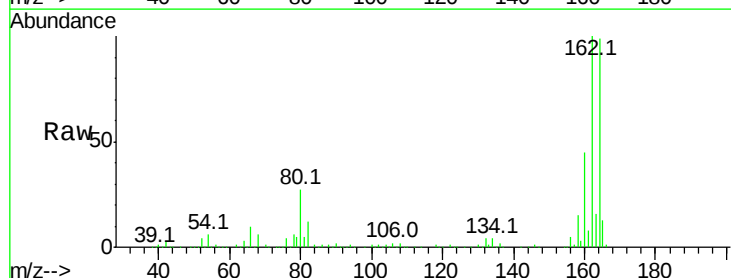


Abundance Ion 164.00 (163.70 to 164.70): BF0

Ion 162.00 (161.70 to 162.70): BF0

Ion 160.00 (159.70 to 160.70): BF0

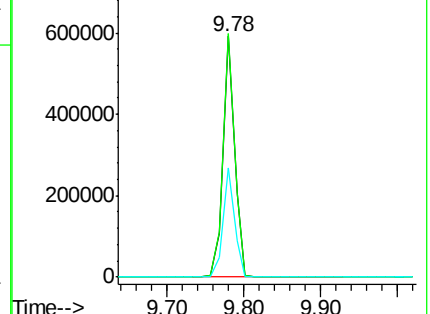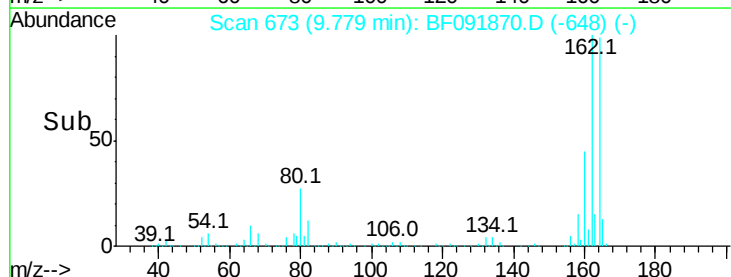


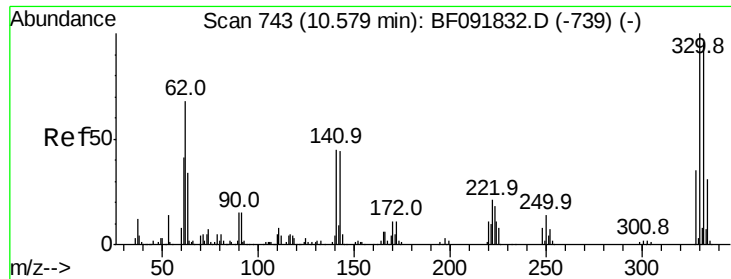




#41
 2,4,6-Tribromophenol
 Concen: 142.20 ng
 RT: 10.58 min Scan# 743
 Delta R.T. -0.00 min
 Lab File: BF091870.D
 Acq: 22 Dec 2016 8:01

Instrument :
 BNA_F
 ClientSampleId :
 MW-12A

Tot Ion:330 Resp: 744083
 Ion Ratio Lower Upper
 330 100
 332 95.4 77.4 116.2
 141 33.3 34.1 51.1#

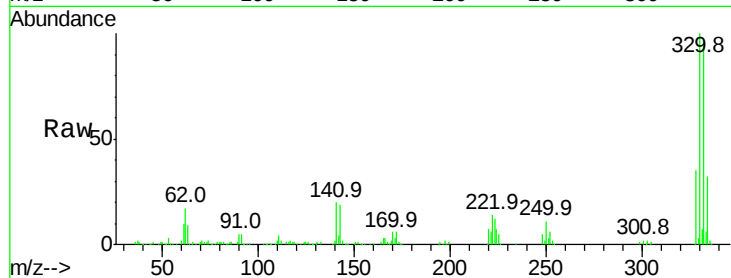


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

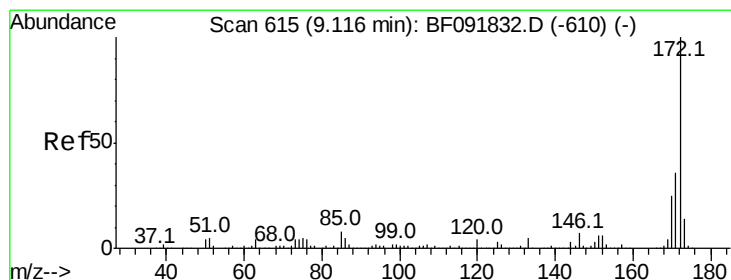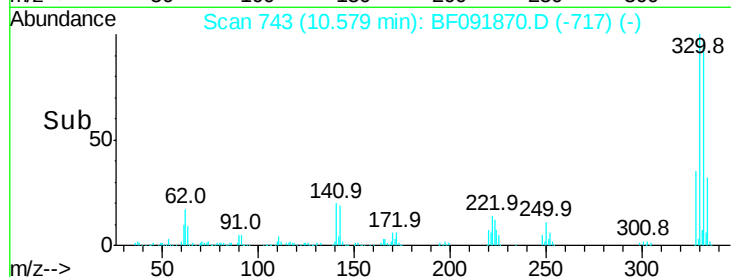
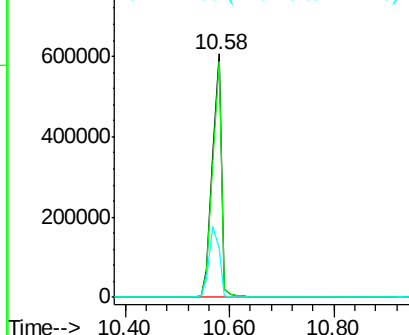



#44
 2-Fluorobiphenyl
 Concen: 109.53 ng
 RT: 9.12 min Scan# 615
 Delta R.T. 0.00 min
 Lab File: BF091870.D
 Acq: 22 Dec 2016 8:01

Tgt Ion:172 Resp: 3265050
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.4 44.0
 170 25.1 20.2 30.4

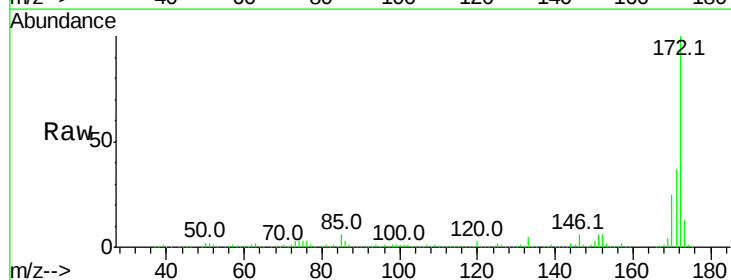

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

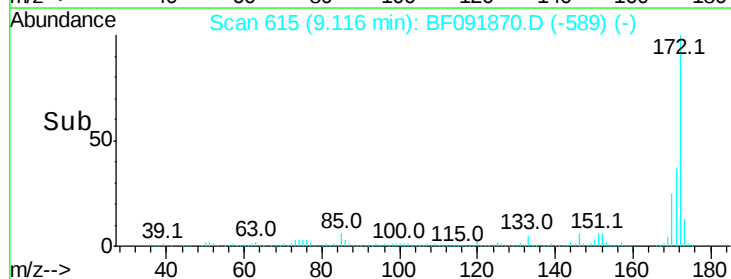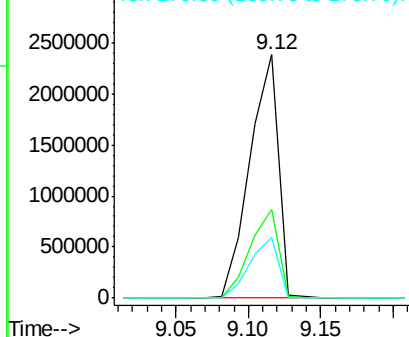


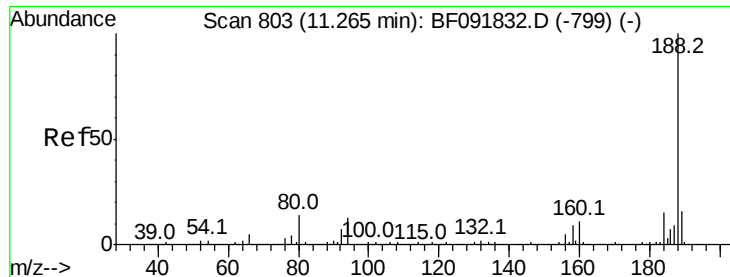




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.26 min Scan# 803
Delta R.T. -0.00 min
Lab File: BF091870.D
Acq: 22 Dec 2016 8:01

Instrument :
BNA_F
ClientSampleId :
MW-12A

Tot Ion:188 Resp: 1082688
Ion Ratio Lower Upper
188 100
94 10.5 10.0 15.0
80 10.7 11.2 16.8#

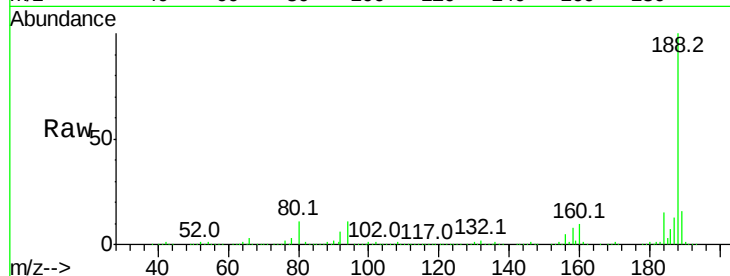


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

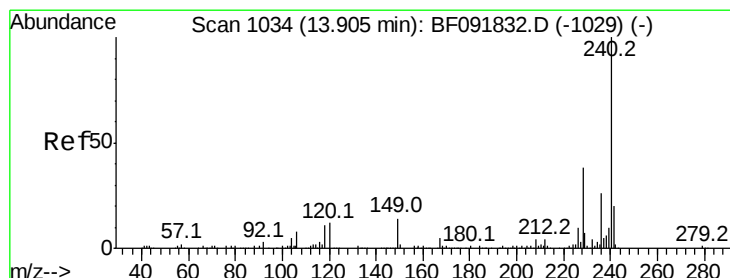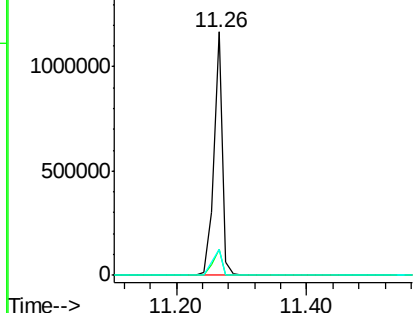
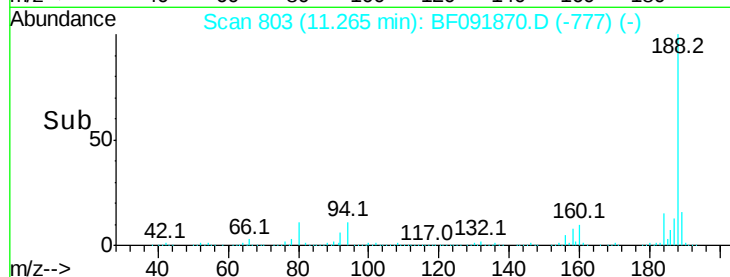



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.89 min Scan# 1033
Delta R.T. -0.01 min
Lab File: BF091870.D
Acq: 22 Dec 2016 8:01

Tgt Ion:240 Resp: 759805
Ion Ratio Lower Upper
240 100
120 14.6 12.9 19.3
236 25.7 20.9 31.3

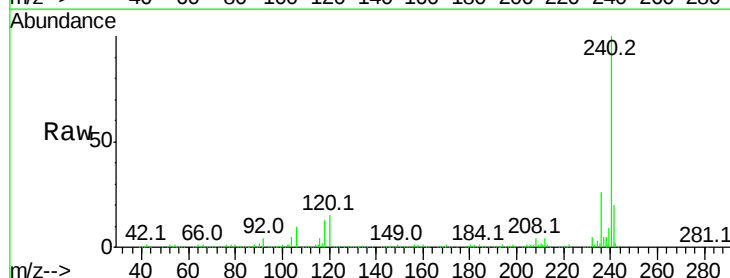

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

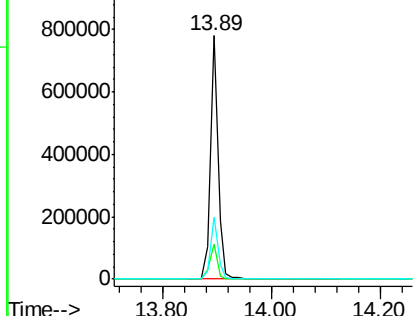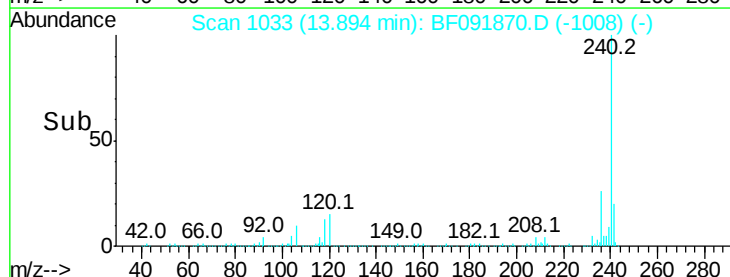

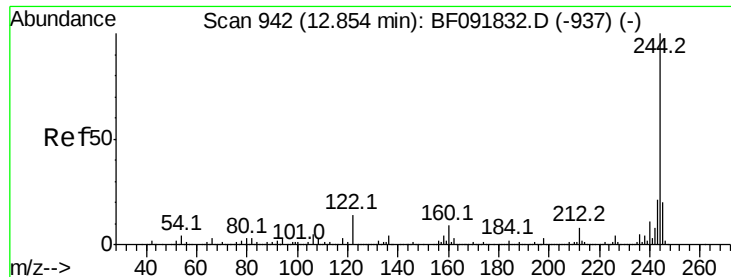

#78

Terphenyl-d14

Concen: 70.53 ng

RT: 12.85 min Scan# 942

Delta R.T. -0.00 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01

Instrument :

BNA_F

ClientSampleId :

MW-12A


Tot Ion:244 Resp: 2209584

Ion Ratio Lower Upper

244 100

212 7.5 6.2 9.2




122 13.7 11.4 17.2

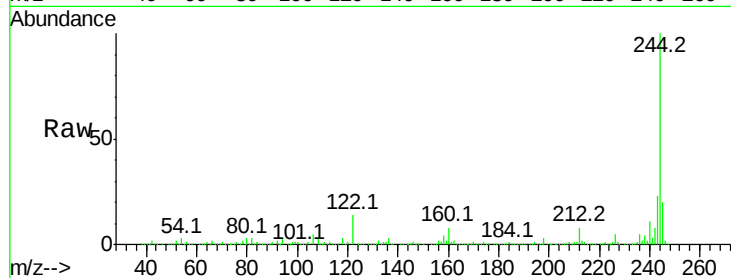

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

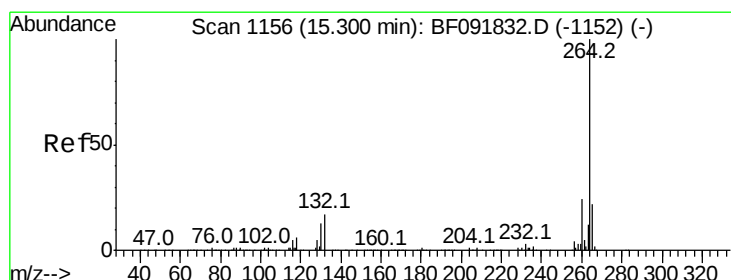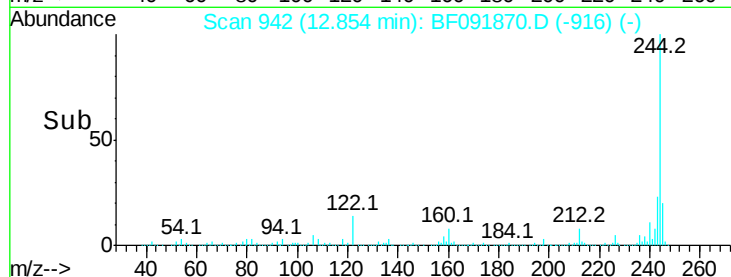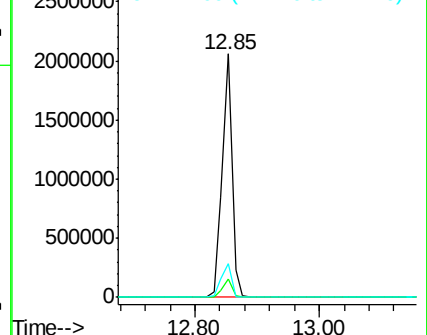

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.29 min Scan# 1155

Delta R.T. -0.01 min

Lab File: BF091870.D

Acq: 22 Dec 2016 8:01


Tgt Ion:264 Resp: 673597

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 21.6 17.4 26.0

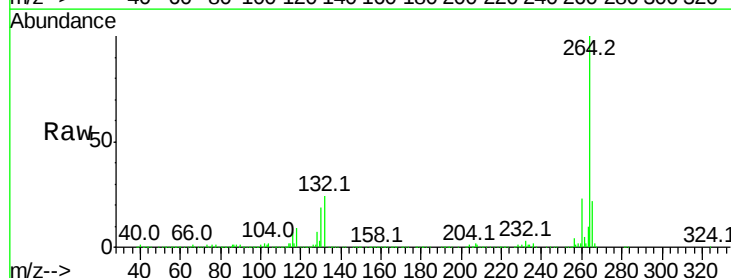

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

