


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122116\
 Data File : BF091828.D
 Acq On : 21 Dec 2016 11:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 16:17:51 2016

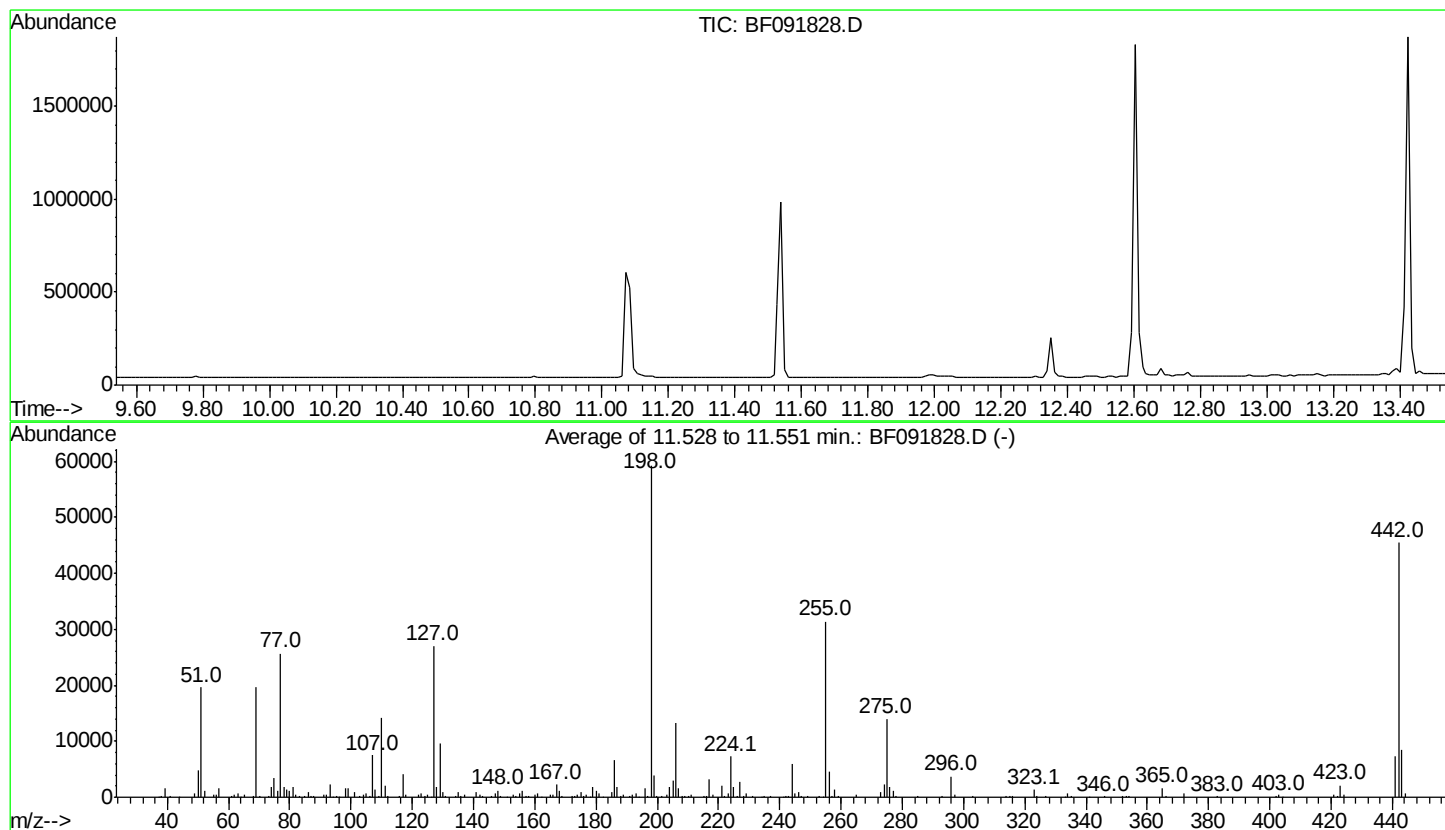

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	19648	PASS
68	69	0.00	2	1.7	341	PASS
69	198	0.00	100	33.3	19753	PASS
70	69	0.00	2	1.1	210	PASS
127	198	10	80	45.7	27058	PASS
197	198	0.00	2	0.5	324	PASS
198	198	100	100	100.0	59239	PASS
199	198	5	9	6.6	3890	PASS
275	198	10	60	23.6	13990	PASS
365	198	1	100	2.7	1616	PASS
441	442	0.01	24	16.2	7373	PASS
442	198	50	100	76.8	45467	PASS
443	442	15	24	18.7	8498	PASS