

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122117\
 Data File : BF101617.D
 Acq On : 21 Dec 2017 19:54
 Operator : SJ/JU
 Sample : I6957-04 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HALSTED-WW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	568	571	587	rBV	29675	82878	10.11%	1.554%
2	6.469	742	745	761	rBV2	31611	97005	11.83%	1.819%
3	6.586	761	765	778	rVB	72234	121031	14.76%	2.270%
4	6.798	797	801	817	rBV	639673	699648	85.32%	13.122%
5	6.957	824	828	836	rBV	72978	94162	11.48%	1.766%
6	7.386	896	901	916	rBV3	26693	65521	7.99%	1.229%
7	8.080	1015	1019	1036	rBV	723316	806553	98.36%	15.126%
8	9.157	1198	1202	1210	rBV	85652	106335	12.97%	1.994%
9	9.574	1262	1273	1276	rBV5	7237	15130	1.85%	0.284%
10	9.751	1300	1303	1306	rBV	8261	8602	1.05%	0.161%
11	9.833	1313	1317	1329	rVB	716413	690669	84.23%	12.953%
12	10.251	1385	1388	1391	rBV	14510	12626	1.54%	0.237%
13	10.451	1418	1422	1428	rBV	73227	68880	8.40%	1.292%
14	10.639	1451	1454	1460	rVB	26734	31957	3.90%	0.599%
15	10.721	1465	1468	1476	rBV3	24159	36587	4.46%	0.686%
16	11.168	1541	1544	1546	rBV	23360	19605	2.39%	0.368%
17	11.198	1546	1549	1553	rVB2	14256	15381	1.88%	0.288%
18	11.321	1567	1570	1579	rBV	676940	666247	81.25%	12.495%
19	11.521	1600	1604	1606	rBV4	6758	10059	1.23%	0.189%
20	11.592	1613	1616	1620	rBV	22956	19319	2.36%	0.362%
21	11.868	1658	1663	1666	rVB3	5434	9593	1.17%	0.180%
22	12.004	1683	1686	1688	rVB	17360	15322	1.87%	0.287%
23	12.062	1693	1696	1701	rVB3	8615	11164	1.36%	0.209%
24	12.386	1746	1751	1755	rBV4	15632	19626	2.39%	0.368%
25	12.492	1767	1769	1772	rBV3	8617	9659	1.18%	0.181%
26	12.762	1812	1815	1817	rBV2	10602	12197	1.49%	0.229%
27	12.904	1836	1839	1843	rVB	123022	105454	12.86%	1.978%
28	13.786	1986	1989	1993	rVB	27574	22129	2.70%	0.415%
29	13.968	2017	2020	2032	rBV	795341	820010	100.00%	15.379%
30	15.439	2265	2270	2280	rVB	475092	638721	77.89%	11.979%


Sum of corrected areas: 5332070

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122117\
Data File : BF101617.D
Acq On : 21 Dec 2017 19:54
Operator : SJ/JU
Sample : I6957-04 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HALSTED-WW

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

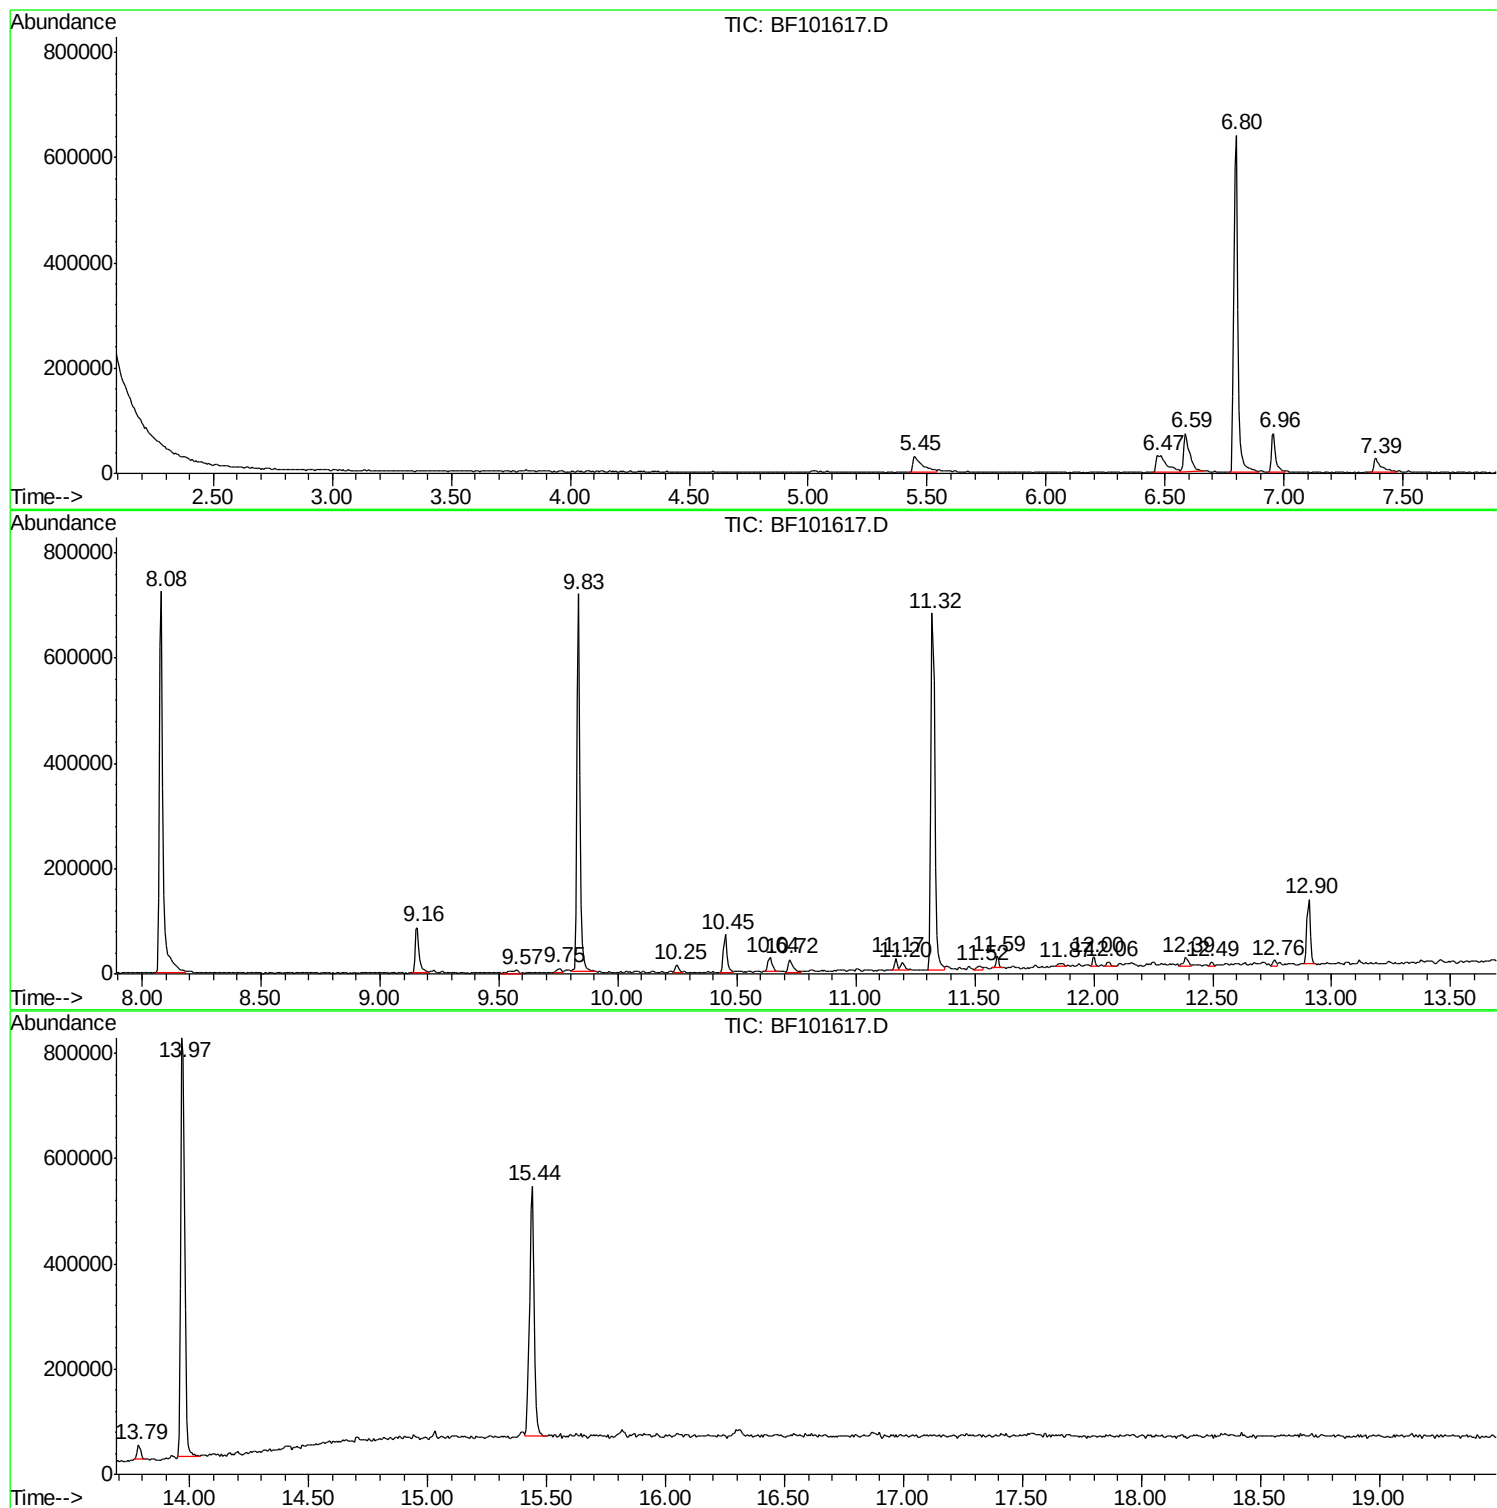

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
Data File : BF101617.D
Acq On : 21 Dec 2017 19:54
Operator : SJ/JU
Sample : I6957-04 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HALSTED-WW










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	3.46 ng	121031	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		2H-Cyclopentaf[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		5-Aminoindole	132	C8H8N2	005192-03-0	9

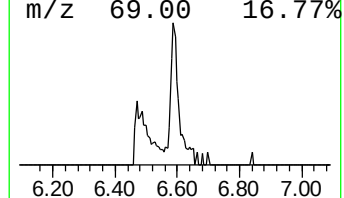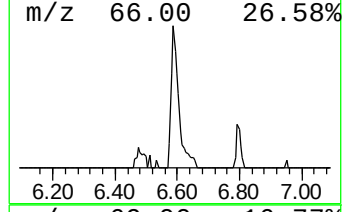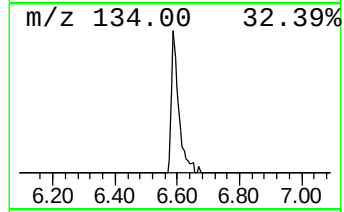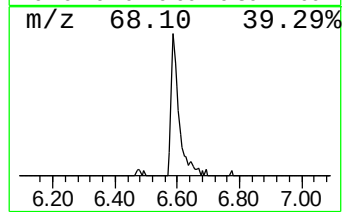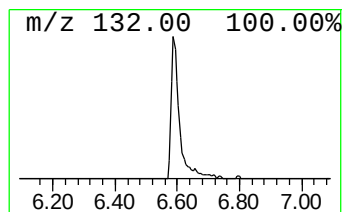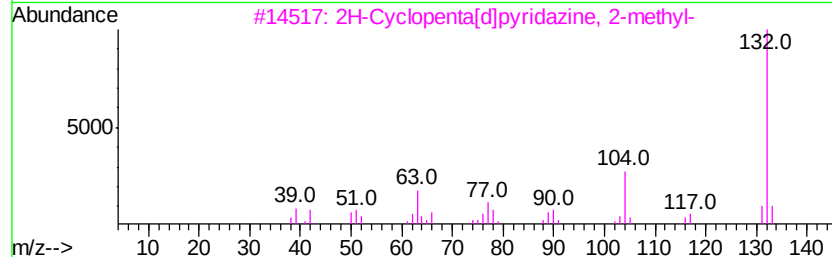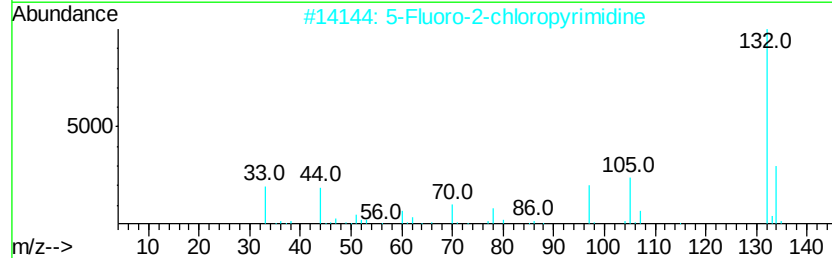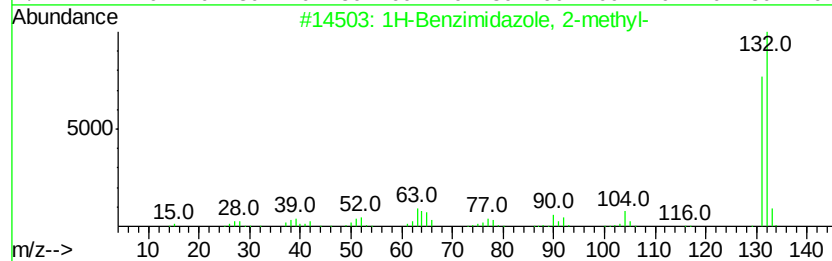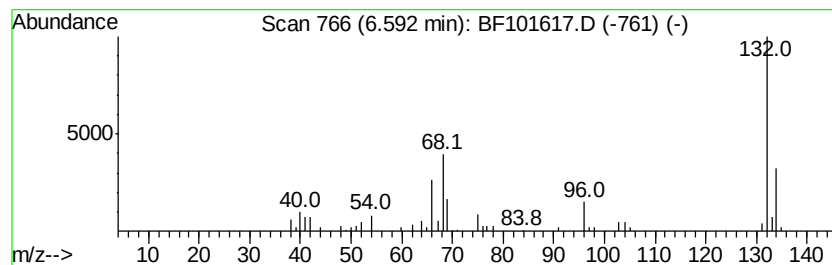

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
Data File : BF101617.D
Acq On : 21 Dec 2017 19:54
Operator : SJ/JU
Sample : I6957-04 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HALSTED-WW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.59	6.59	3.5	ng	121031	1	6.80	699648	20.0