

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122117\
 Data File : BF101629.D
 Acq On : 22 Dec 2017 2:41
 Operator : SJ/JU
 Sample : I6971-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 121517-TIFR-E-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	495	498	510	rBV	28226	56517	1.79%	0.268%
2	5.416	563	566	587	rBV	819906	1295059	41.10%	6.135%
3	6.439	737	740	758	rBV	523827	860342	27.31%	4.075%
4	6.569	758	762	769	rBV	1919975	1981871	62.90%	9.388%
5	6.792	797	800	810	rBV	769383	809453	25.69%	3.834%
6	6.951	823	827	843	rBV	2655488	2573371	81.68%	12.190%
7	7.363	893	897	916	rBV	1852469	2157607	68.48%	10.220%
8	8.075	1015	1018	1033	rBV	883137	974875	30.94%	4.618%
9	9.151	1197	1201	1204	rBV	3408618	3150683	100.00%	14.924%
10	9.833	1313	1317	1327	rVB	820990	856959	27.20%	4.059%
11	10.627	1448	1452	1465	rBV	930806	1048774	33.29%	4.968%
12	11.322	1567	1570	1580	rBV	761487	732958	23.26%	3.472%
13	12.710	1802	1806	1809	rBV	170118	148772	4.72%	0.705%
14	12.786	1816	1819	1823	rVB	40784	35130	1.11%	0.166%
15	12.904	1835	1839	1842	rBV	2678505	2434823	77.28%	11.533%
16	13.410	1922	1925	1929	rBV	119288	109174	3.47%	0.517%
17	13.786	1986	1989	2003	rVB2	38978	67608	2.15%	0.320%
18	13.968	2016	2020	2030	rBV	909553	862930	27.39%	4.088%
19	14.098	2038	2042	2048	rBV	33473	34069	1.08%	0.161%
20	14.404	2089	2094	2098	rBV	37835	36411	1.16%	0.172%
21	14.704	2141	2145	2148	rBV	43624	40121	1.27%	0.190%
22	15.027	2197	2200	2205	rBV	37729	43022	1.37%	0.204%
23	15.398	2258	2263	2265	rBV2	33385	42081	1.34%	0.199%
24	15.433	2265	2269	2284	rVB	473343	676870	21.48%	3.206%
25	15.815	2330	2334	2339	rVB2	25671	38443	1.22%	0.182%
26	16.298	2412	2416	2424	rBV4	24018	42974	1.36%	0.204%


Sum of corrected areas: 21110897

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
Data File : BF101629.D
Acq On : 22 Dec 2017 2:41
Operator : SJ/JU
Sample : I6971-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
121517-TIFR-E-U-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

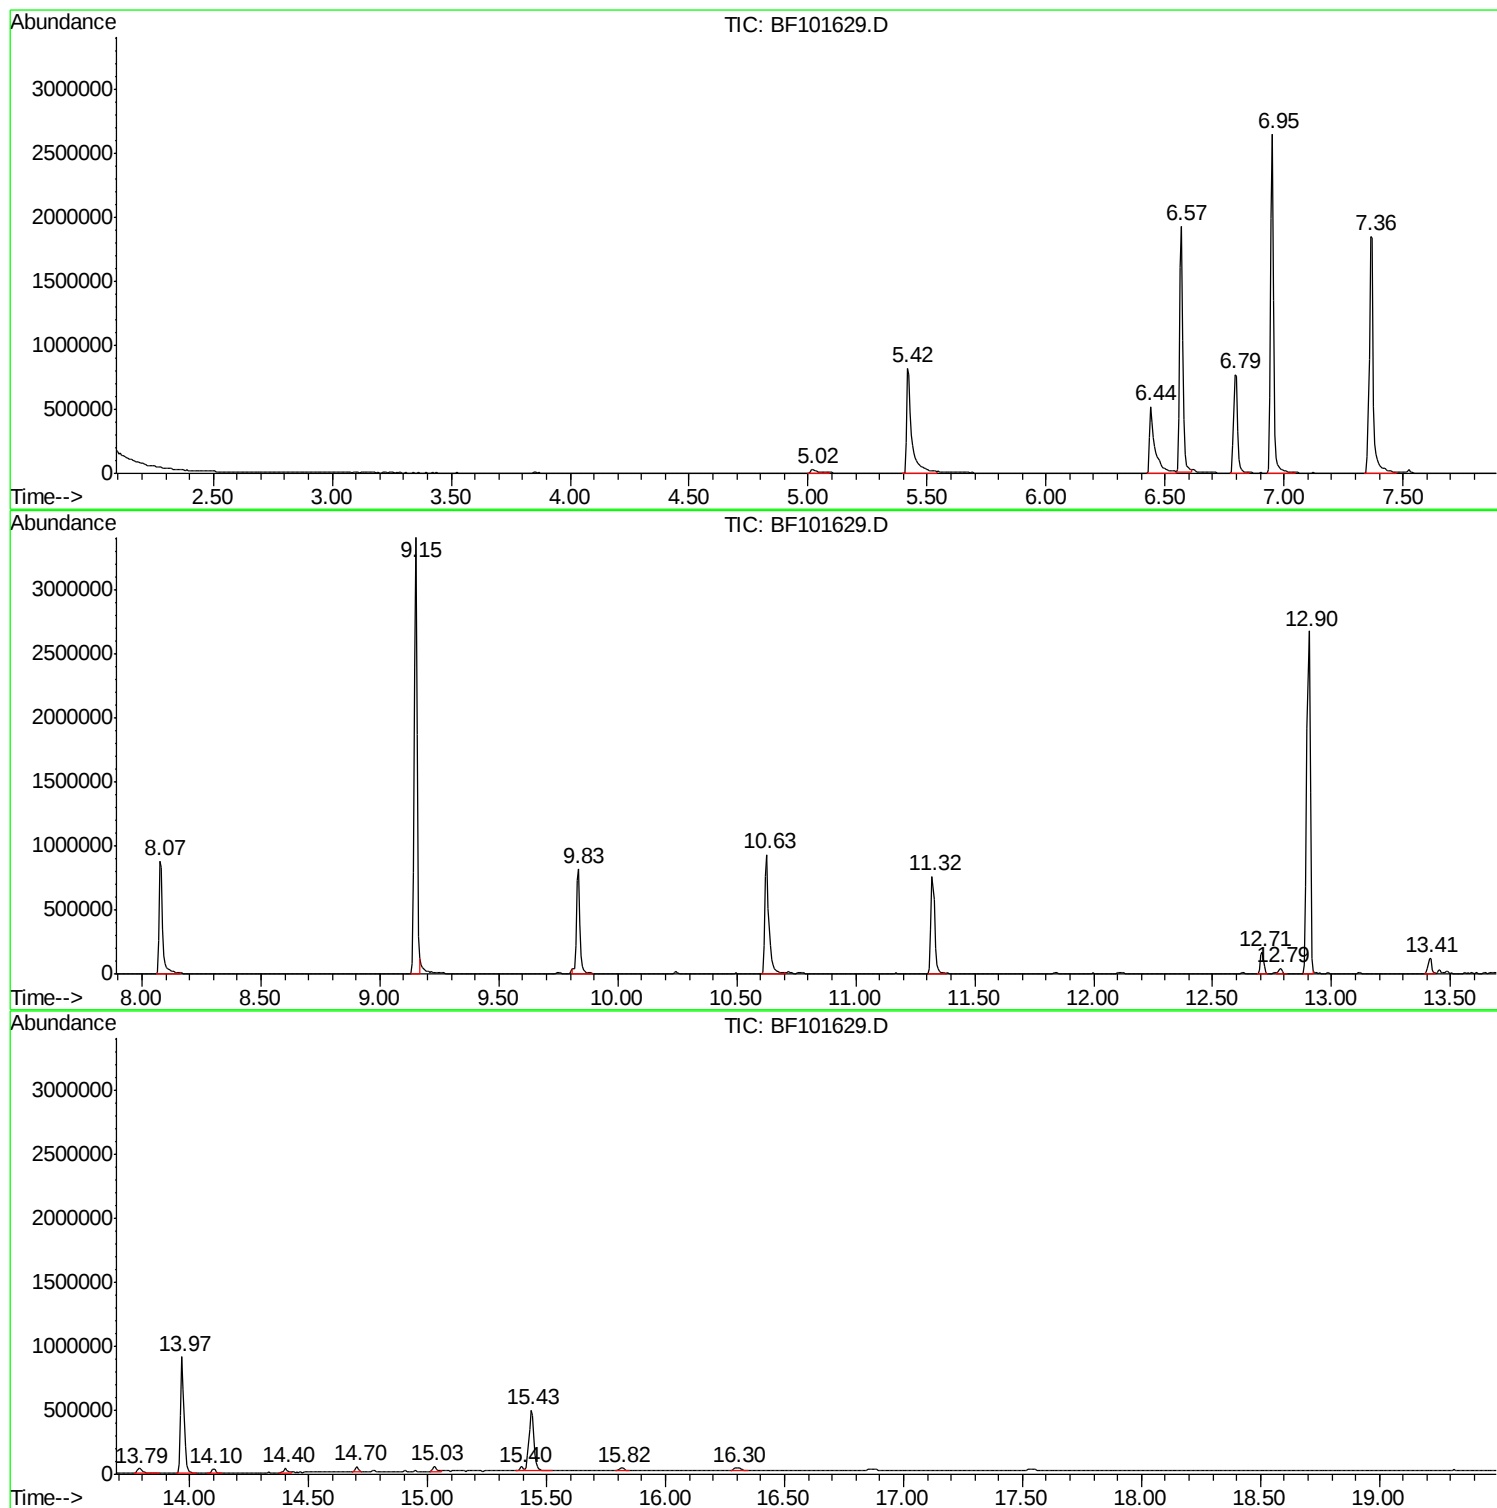

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
Data_File : BF101629.D
Acq_On : 22-Dec-2017 2:411
Operator : SJ/JUU
Sample : I6971-199
Misc :
ALS_Vial : 31 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
121517-TIFR-E-U-M

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
