

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122117\
 Data File : BF101643.D
 Acq On : 22 Dec 2017 8:55
 Operator : SJ/JU
 Sample : I6681-07DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-01-121917-DDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.004	493	496	510	rBV	61411	109525	4.78%	0.305%
2	5.422	563	567	587	rBV	351303	665936	29.04%	1.856%
3	6.440	737	740	759	rBV	368104	729447	31.81%	2.033%
4	6.569	759	762	778	rVB	663263	739506	32.25%	2.061%
5	6.792	797	800	816	rVB	766217	826415	36.04%	2.303%
6	6.951	823	827	838	rBV	545280	553350	24.13%	1.542%
7	7.369	895	898	916	rBV	274061	409208	17.85%	1.140%
8	8.081	1015	1019	1021	rBV	1045679	1052099	45.89%	2.932%
9	8.098	1021	1022	1030	rVB	550309	452432	19.73%	1.261%
10	8.792	1137	1140	1148	rBV	485868	443953	19.36%	1.237%
11	8.892	1153	1157	1166	rVB	378512	367146	16.01%	1.023%
12	9.151	1197	1201	1209	rBV	824971	724677	31.61%	2.019%
13	9.257	1216	1219	1224	rBV	72916	68792	3.00%	0.192%
14	9.351	1233	1235	1242	rVB	76839	86254	3.76%	0.240%
15	9.422	1242	1247	1251	rBV	158100	220714	9.63%	0.615%
16	9.492	1255	1259	1261	rVV	267228	275877	12.03%	0.769%
17	9.522	1261	1264	1267	rVV	162534	172168	7.51%	0.480%
18	9.610	1276	1279	1287	rVB	127212	158431	6.91%	0.441%
19	9.698	1290	1294	1299	rBV2	126025	133677	5.83%	0.372%
20	9.833	1310	1317	1320	rBV	1089013	1011579	44.12%	2.819%
21	9.863	1320	1322	1331	rVB	392398	403430	17.60%	1.124%
22	9.939	1331	1335	1339	rBV2	53484	77099	3.36%	0.215%
23	10.039	1348	1352	1355	rVV2	162549	196057	8.55%	0.546%
24	10.075	1355	1358	1362	rVB	107394	96501	4.21%	0.269%
25	10.145	1367	1370	1373	rBV	80969	88043	3.84%	0.245%
26	10.239	1381	1386	1392	rBV3	60898	121073	5.28%	0.337%
27	10.380	1407	1410	1416	rVV	515763	496808	21.67%	1.384%
28	10.445	1419	1421	1423	rVV	103682	105081	4.58%	0.293%
29	10.469	1423	1425	1427	rVV	102237	86928	3.79%	0.242%
30	10.539	1435	1437	1440	rVB2	85444	77610	3.38%	0.216%
31	10.633	1447	1453	1458	rBV2	252758	339477	14.81%	0.946%
32	10.933	1496	1504	1506	rBV	168158	219144	9.56%	0.611%
33	10.957	1506	1508	1511	rVV	107309	111726	4.87%	0.311%
34	11.010	1514	1517	1520	rVV	100383	105002	4.58%	0.293%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
 Data File : BF101643.D
 Acq On : 22 Dec 2017 8:55
 Operator : SJ/JU
 Sample : I6681-07DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-01-121917-DDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.080	1527	1529	1534	rVV2	66113	84775	3.70%	0.236%
36	11.139	1534	1539	1542	rVV4	40303	80172	3.50%	0.223%
37	11.169	1542	1544	1548	rVV3	77982	91546	3.99%	0.255%
38	11.222	1550	1553	1560	rVB	196745	179018	7.81%	0.499%
39	11.322	1567	1570	1572	rBV2	852569	780953	34.06%	2.176%
40	11.351	1572	1575	1578	rVV	1899435	1668112	72.75%	4.648%
41	11.404	1580	1584	1589	rBV	594443	579258	25.26%	1.614%
42	11.563	1606	1611	1615	rVV2	96323	125720	5.48%	0.350%
43	11.657	1622	1627	1632	rBV	127900	141372	6.17%	0.394%
44	11.739	1638	1641	1646	rVB2	77548	104491	4.56%	0.291%
45	11.822	1652	1655	1658	rVV	505693	474598	20.70%	1.322%
46	11.857	1658	1661	1665	rVV	562583	526779	22.98%	1.468%
47	11.904	1666	1669	1671	rVV	243006	202710	8.84%	0.565%
48	11.939	1671	1675	1677	rVV2	680743	752074	32.80%	2.096%
49	11.963	1677	1679	1683	rVB	345073	294835	12.86%	0.822%
50	12.116	1702	1705	1710	rBV	205600	216912	9.46%	0.604%
51	12.169	1710	1714	1716	rVB3	64364	71923	3.14%	0.200%
52	12.269	1729	1731	1734	rVB	104925	77037	3.36%	0.215%
53	12.298	1734	1736	1739	rBV	117133	100614	4.39%	0.280%
54	12.327	1739	1741	1744	rVB	89380	70832	3.09%	0.197%
55	12.374	1744	1749	1752	rBV	362038	395209	17.24%	1.101%
56	12.416	1752	1756	1758	rVV2	118440	140654	6.13%	0.392%
57	12.474	1764	1766	1773	rVB2	174360	221984	9.68%	0.619%
58	12.539	1773	1777	1781	rBV	1731954	1714332	74.77%	4.777%
59	12.580	1781	1784	1786	rVV2	82135	80617	3.52%	0.225%
60	12.604	1786	1788	1792	rVB2	91119	89262	3.89%	0.249%
61	12.692	1800	1803	1805	rBV	162573	152717	6.66%	0.426%
62	12.774	1810	1817	1822	rBV	2010240	2292816	100.00%	6.389%
63	12.821	1822	1825	1828	rVB	135253	129567	5.65%	0.361%
64	12.904	1835	1839	1841	rBV2	528978	502431	21.91%	1.400%
65	12.992	1849	1854	1858	rBV3	255357	403744	17.61%	1.125%
66	13.039	1858	1862	1865	rVV3	61047	83578	3.65%	0.233%
67	13.074	1865	1868	1870	rVV3	185932	257506	11.23%	0.718%
68	13.098	1870	1872	1877	rVB	481034	462761	20.18%	1.290%
69	13.163	1880	1883	1886	rVV	403345	357412	15.59%	0.996%
70	13.204	1886	1890	1894	rVV	444394	484609	21.14%	1.350%
71	13.298	1903	1906	1908	rVV	299679	256526	11.19%	0.715%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122117\
 Data File : BF101643.D
 Acq On : 22 Dec 2017 8:55
 Operator : SJ/JU
 Sample : I6681-07DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-01-121917-DDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.327	1908	1911	1920	rVB	325399	374233	16.32%	1.043%
73	13.410	1920	1925	1929	rBV3	52808	92773	4.05%	0.259%
74	13.469	1929	1935	1937	rBV6	45235	78964	3.44%	0.220%
75	13.504	1937	1941	1942	rBV	75949	81737	3.56%	0.228%
76	13.580	1951	1954	1957	rBV2	93972	125260	5.46%	0.349%
77	13.616	1957	1960	1963	rVV2	135742	169198	7.38%	0.471%
78	13.721	1972	1978	1980	rBV2	248614	328239	14.32%	0.915%
79	13.745	1980	1982	1984	rVV	229601	189614	8.27%	0.528%
80	13.774	1984	1987	1994	rVV3	155120	289140	12.61%	0.806%
81	13.833	1994	1997	2002	rVB2	144518	181056	7.90%	0.505%
82	13.968	2015	2020	2023	rBV2	1267611	1998040	87.14%	5.568%
83	13.998	2023	2025	2031	rVB	1111185	980533	42.77%	2.732%
84	14.080	2036	2039	2041	rVB	188020	146468	6.39%	0.408%
85	14.133	2045	2048	2053	rBV2	134942	160507	7.00%	0.447%
86	14.321	2077	2080	2082	rBV	105387	90708	3.96%	0.253%
87	14.357	2082	2086	2090	rVV	333083	393454	17.16%	1.096%
88	14.392	2090	2092	2096	rVB	176319	141758	6.18%	0.395%
89	14.433	2096	2099	2101	rBV2	106176	109609	4.78%	0.305%
90	14.457	2101	2103	2106	rVB2	115396	105503	4.60%	0.294%
91	14.486	2106	2108	2110	rBV2	179971	182443	7.96%	0.508%
92	14.857	2168	2171	2174	rBV2	71905	89480	3.90%	0.249%
93	15.015	2194	2198	2201	rBV	547686	842129	36.73%	2.347%
94	15.121	2213	2216	2220	rBV	113293	129083	5.63%	0.360%
95	15.315	2245	2249	2255	rVB	380940	421077	18.37%	1.173%
96	15.380	2256	2260	2266	rVV	495959	636469	27.76%	1.774%
97	15.439	2266	2270	2273	rVV	449319	519369	22.65%	1.447%
98	15.468	2273	2275	2281	rVB3	109083	154273	6.73%	0.430%
99	16.921	2518	2522	2529	rVB2	146610	256438	11.18%	0.715%
100	17.362	2594	2597	2607	rVB	120564	244280	10.65%	0.681%


Sum of corrected areas: 35886456

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
Data File : BF101643.D
Acq On : 22 Dec 2017 8:55
Operator : SJ/JU
Sample : I6681-07DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-01-121917-DDL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

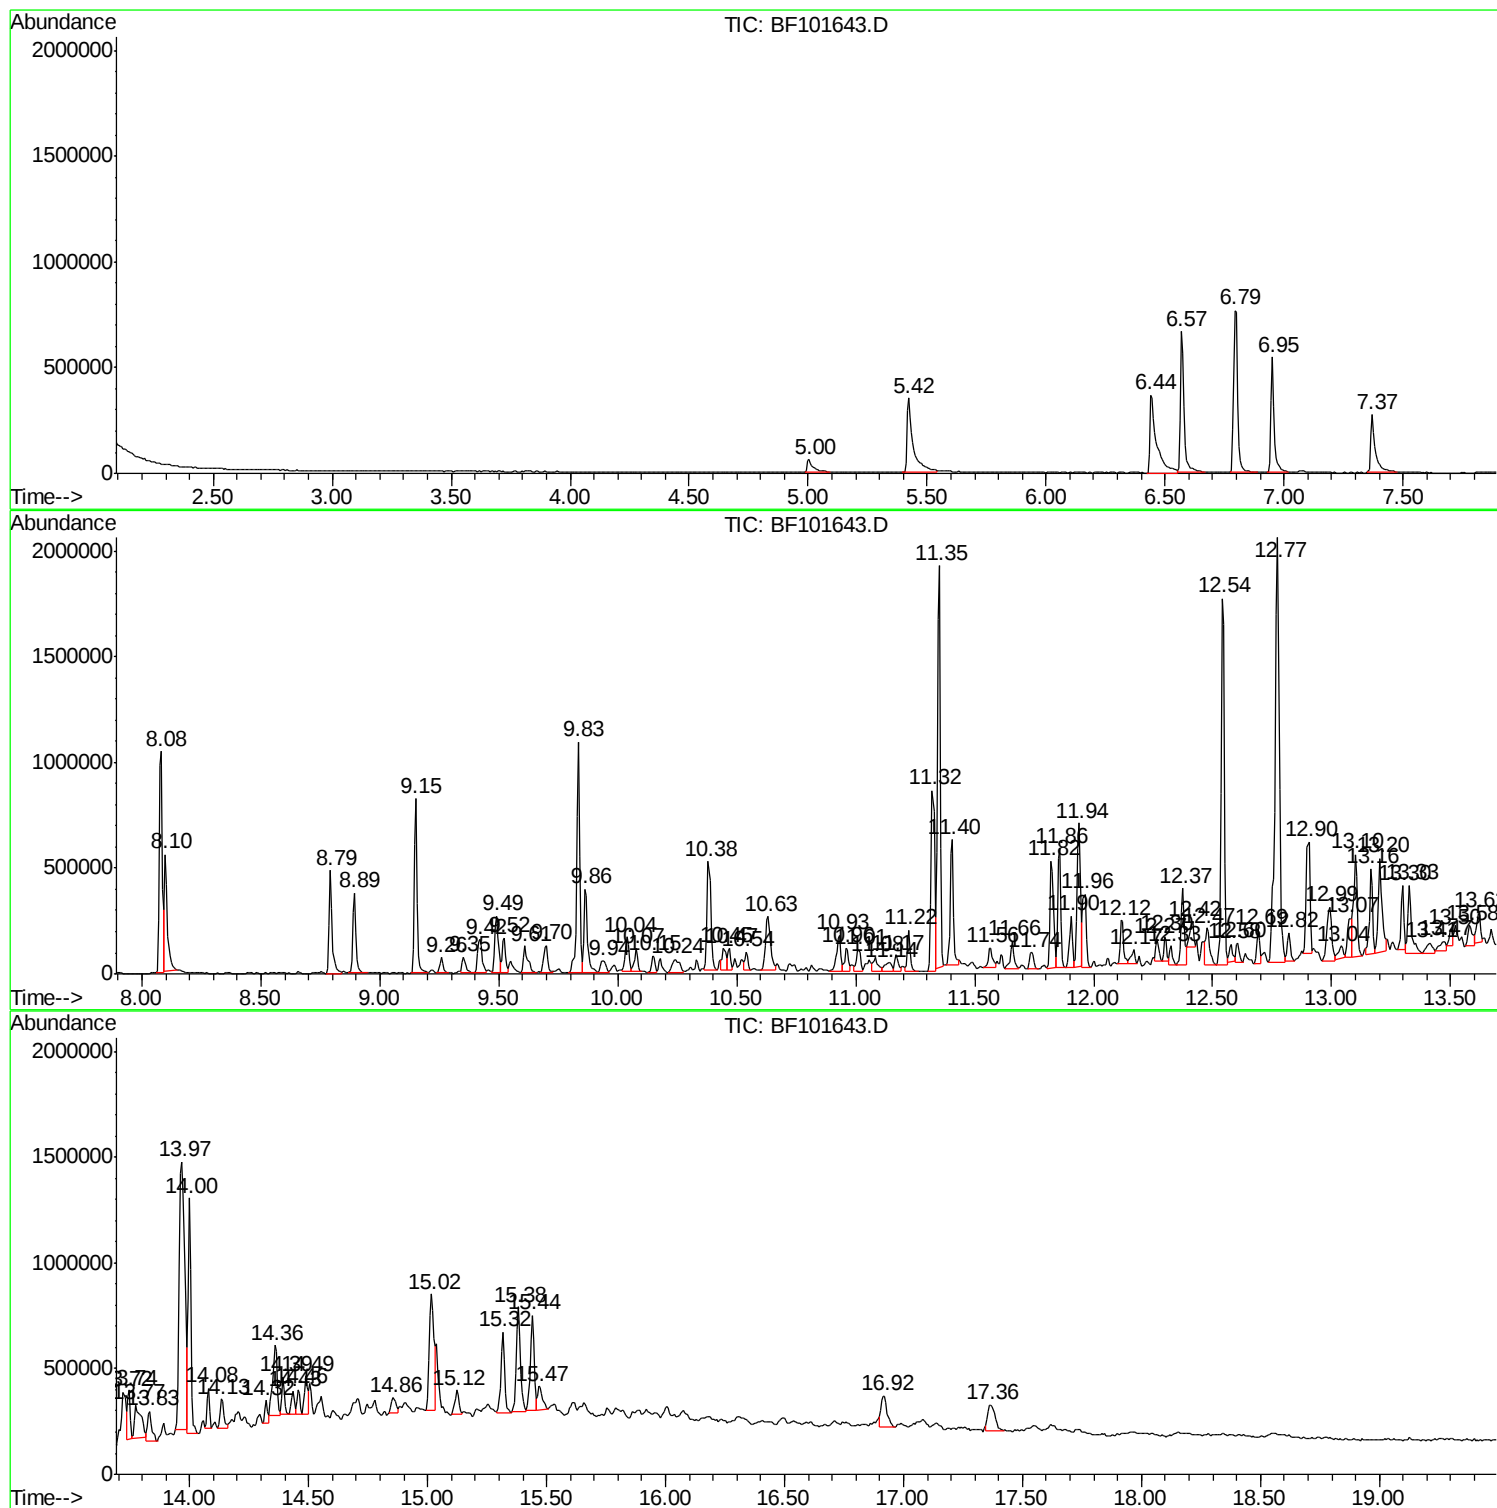

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF122117\
Data_File : BF101643.D
Acq_On : 22-Dec-2017 8:555
Operator : SJ/JUU
Sample : I6681-07DL_5XX
Misc :
ALS_Vial : 45 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PL-01-121917-DDL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
