


Data Path : Z:\HPCHEM1\BNA F\Data\BF122117\
 Data File : BF101623.D
 Acq On : 21 Dec 2017 23:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 16:07:58 2017

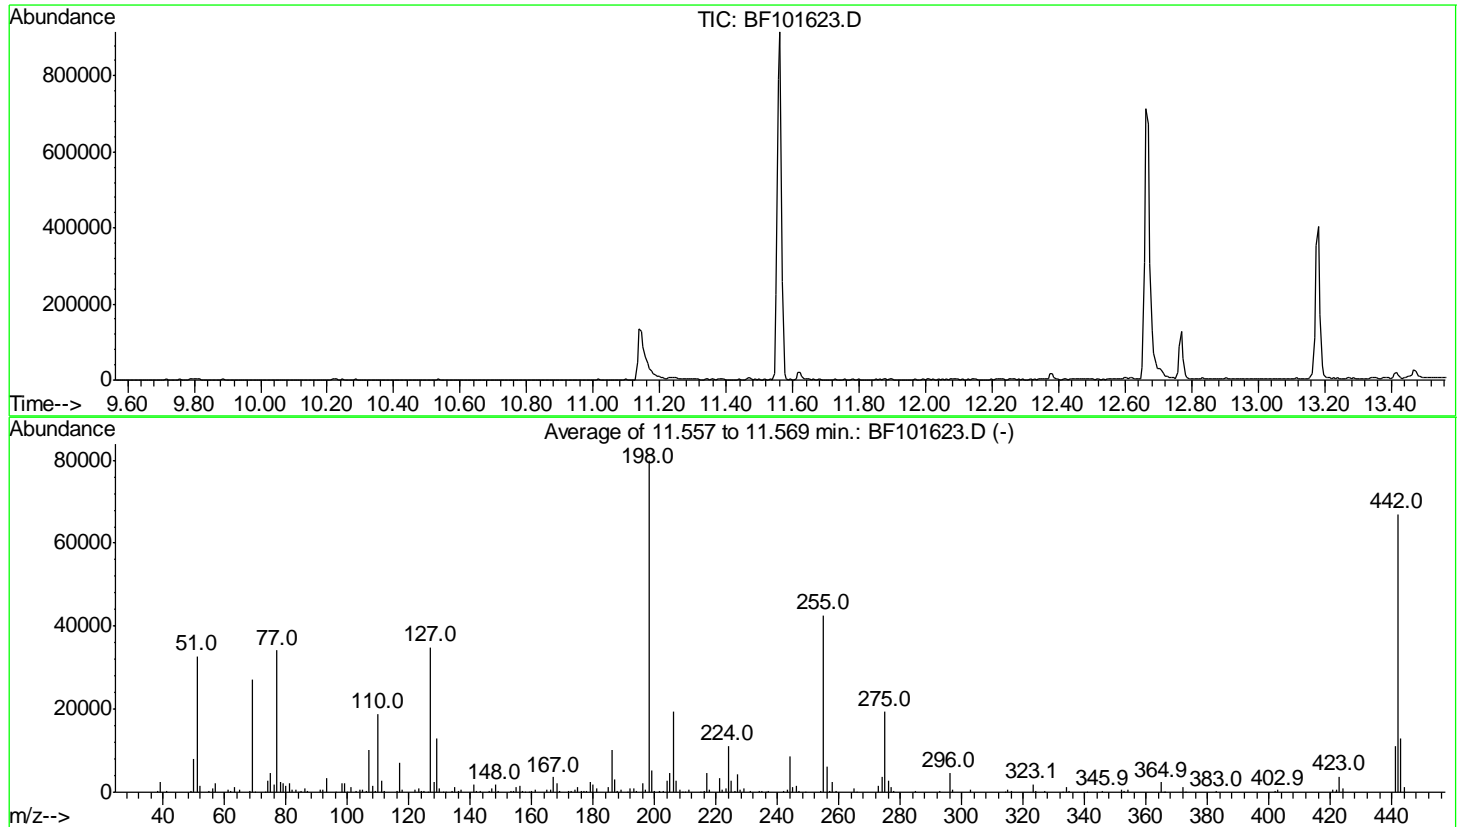

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	32792	PASS
68	69	0.00	2	1.5	421	PASS
69	198	0.00	100	34.0	27184	PASS
70	69	0.00	2	0.5	126	PASS
127	198	10	80	43.7	34908	PASS
197	198	0.00	2	1.0	768	PASS
198	198	100	100	100.0	79893	PASS
199	198	5	9	6.5	5229	PASS
275	198	10	60	24.2	19349	PASS
365	198	1	100	3.0	2429	PASS
441	443	0.01	100	86.6	11128	PASS
442	198	50	100	83.8	66978	PASS
443	442	15	24	19.2	12855	PASS