

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122120\
 Data File : BF122800.D
 Acq On : 21 Dec 2020 14:41
 Operator : JU/CG
 Sample : PB133720BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133720BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	567	572	575	rBV	4066860	4364820	64.68%	11.496%
2	6.457	737	743	746	rBV	3666523	4286057	63.51%	11.289%
3	6.816	800	804	808	rBV	1379385	1115345	16.53%	2.938%
4	7.381	895	900	904	rBV	2496338	3039755	45.04%	8.006%
5	8.098	1017	1022	1026	rBV	1415478	1490393	22.08%	3.925%
6	9.181	1199	1206	1209	rBV	4773487	5483333	81.25%	14.442%
7	9.857	1315	1321	1343	rBV	1898046	1816639	26.92%	4.785%
8	10.651	1449	1456	1478	rBV	3213706	3884186	57.55%	10.230%
9	11.345	1568	1574	1581	rBV	1921017	1876280	27.80%	4.942%
10	12.939	1836	1845	1848	rBV	5557465	6748698	100.00%	17.775%
11	13.986	2019	2023	2036	rBV	1862346	1902902	28.20%	5.012%
12	15.445	2266	2271	2292	rBV	1199644	1881408	27.88%	4.955%
13	16.757	2482	2494	2496	rBV5	23282	77274	1.15%	0.204%




Sum of corrected areas: 37967090

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122120\
Data File : BF122800.D
Acq On : 21 Dec 2020 14:41
Operator : JU/CG
Sample : PB133720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

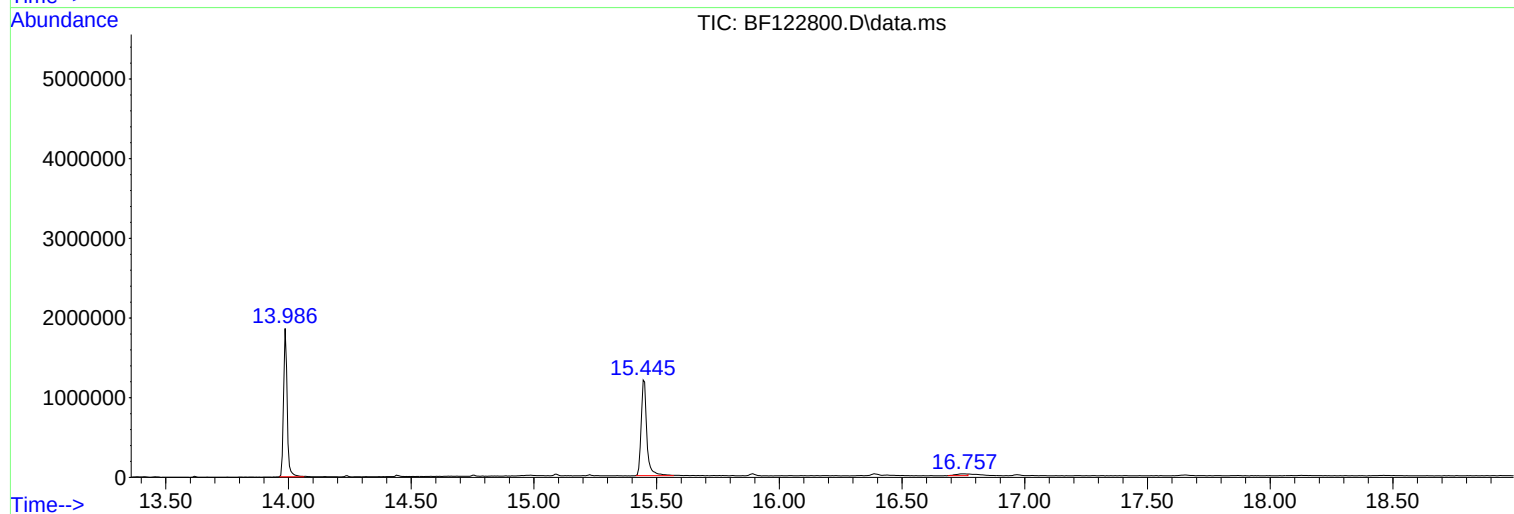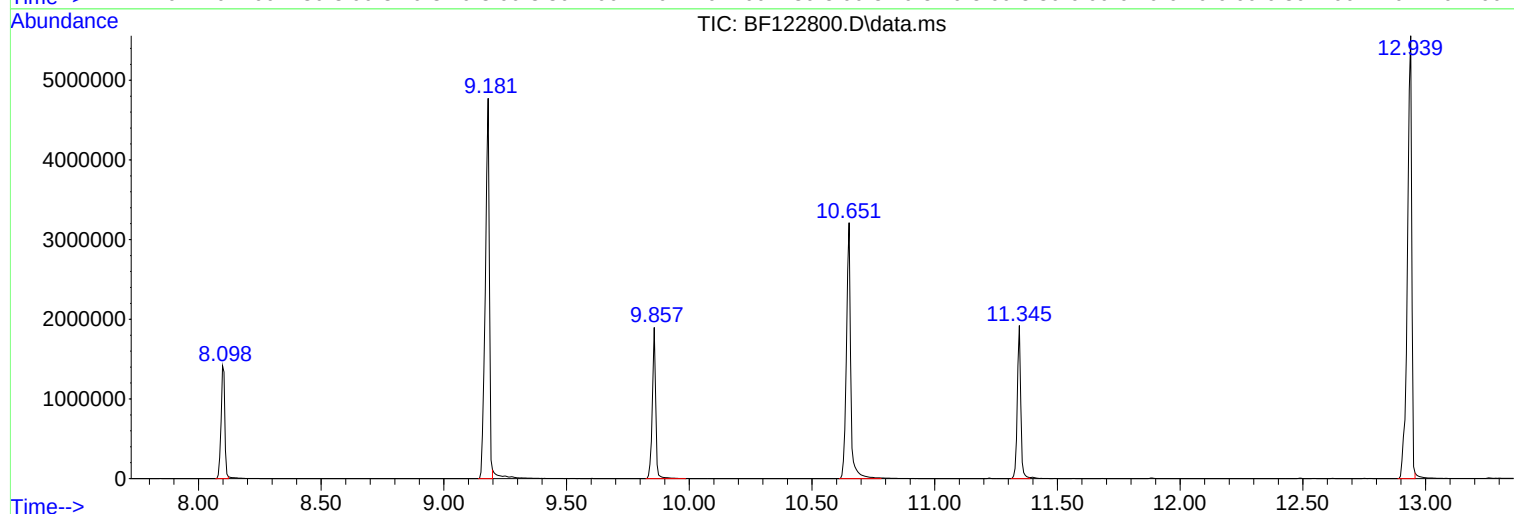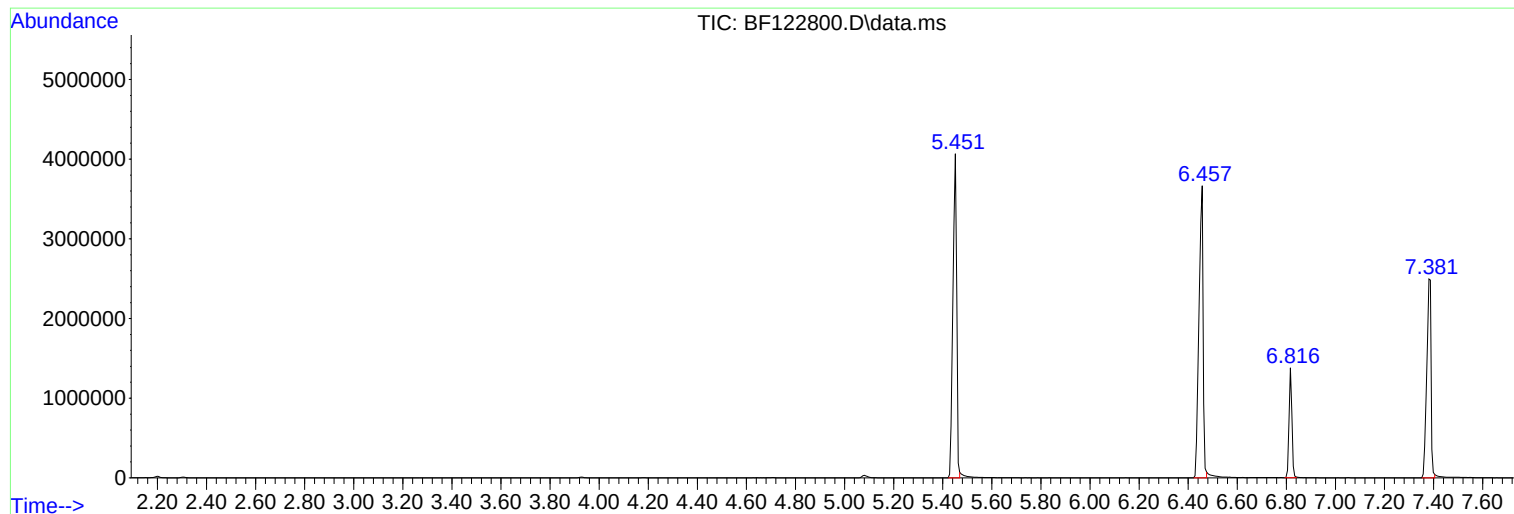

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122120\
Data File : BF122800.D
Acq On : 21 Dec 2020 14:41
Operator : JU/CG
Sample : PB133720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122120\
Data File : BF122800.D
Acq On : 21 Dec 2020 14:41
Operator : JU/CG
Sample : PB133720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------