
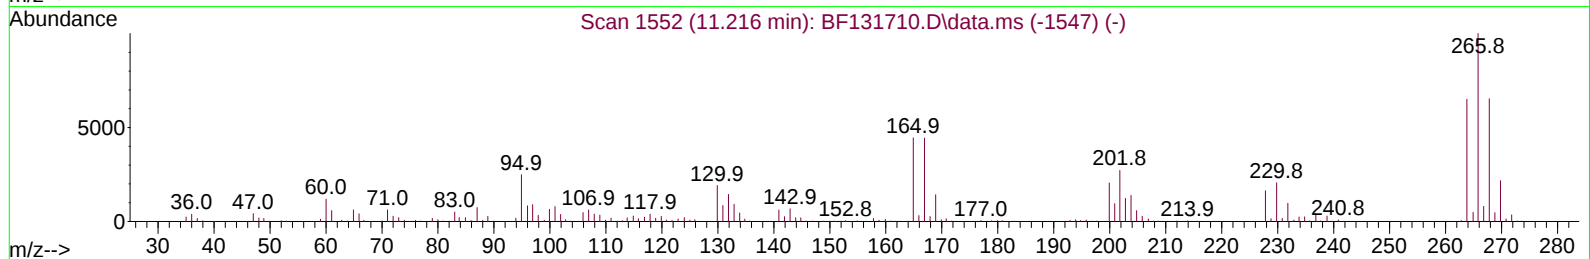
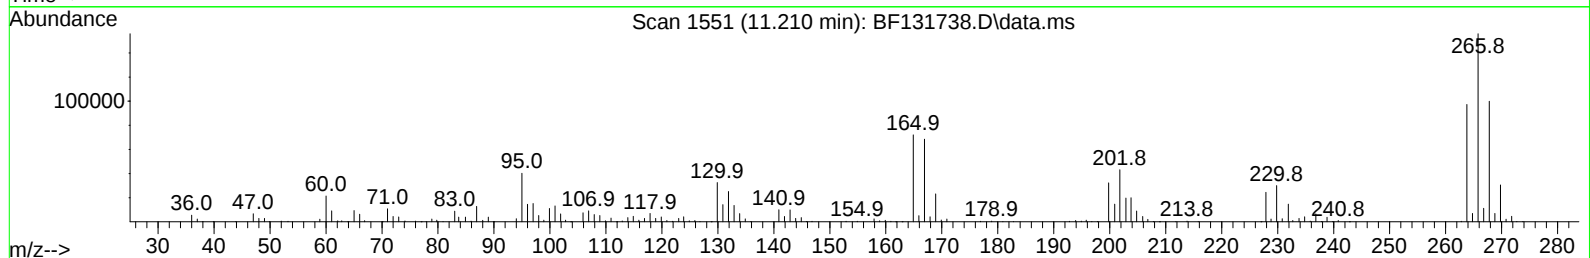


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
Data File : BF131738.D
Acq On : 21 Dec 2022 09:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 08:12:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration



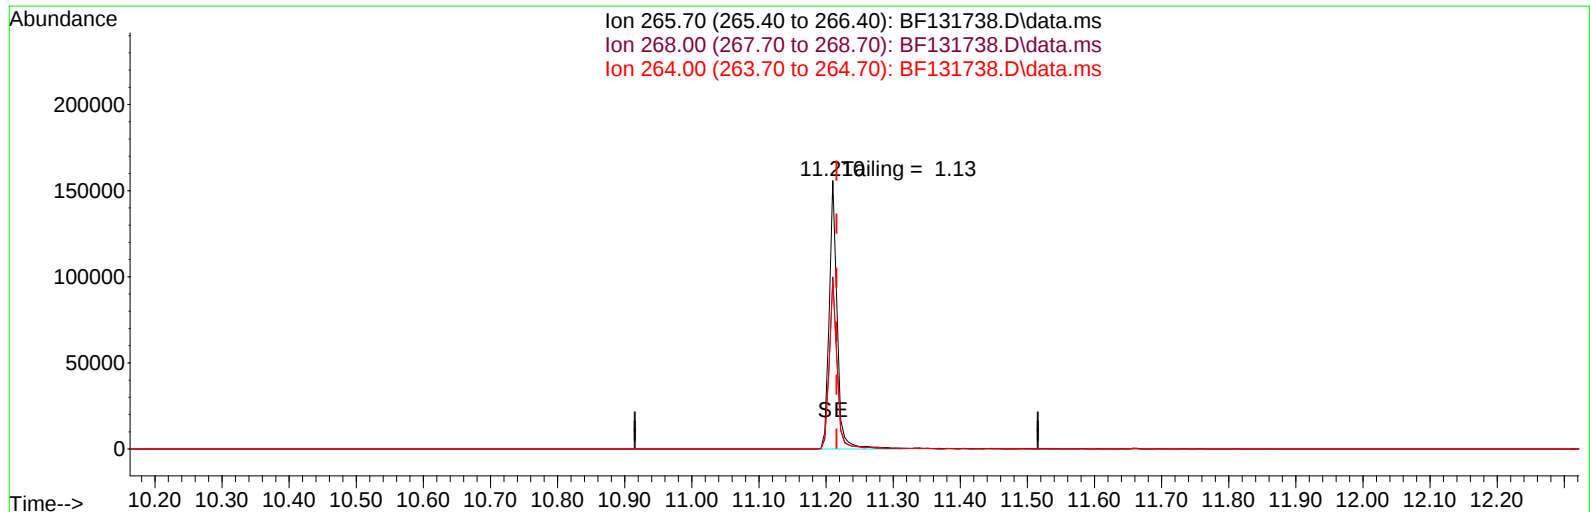


TIC: BF131738.D\data.ms

(70) Pentachlorophenol (C)**11.210min (-0.006) 30620.82 ng****response 129831**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.10
264.00	65.00	62.42
0.00	0.00	0.00

Quant Time: Dec 22 08:12:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

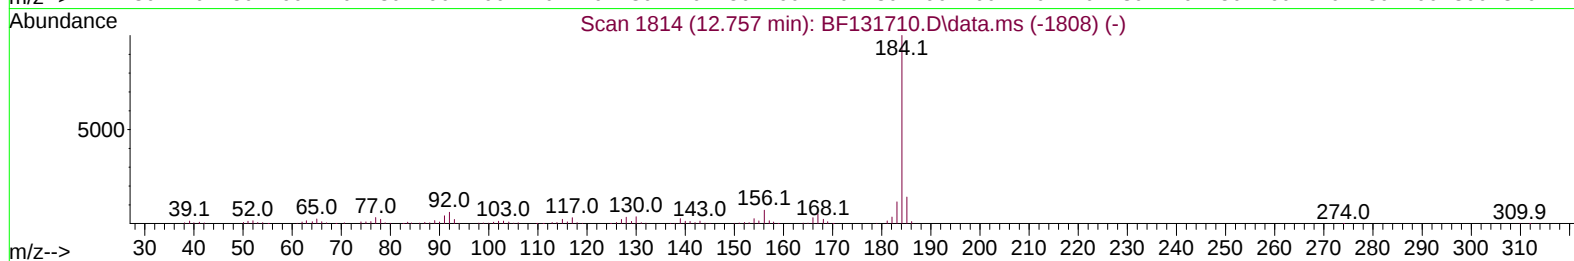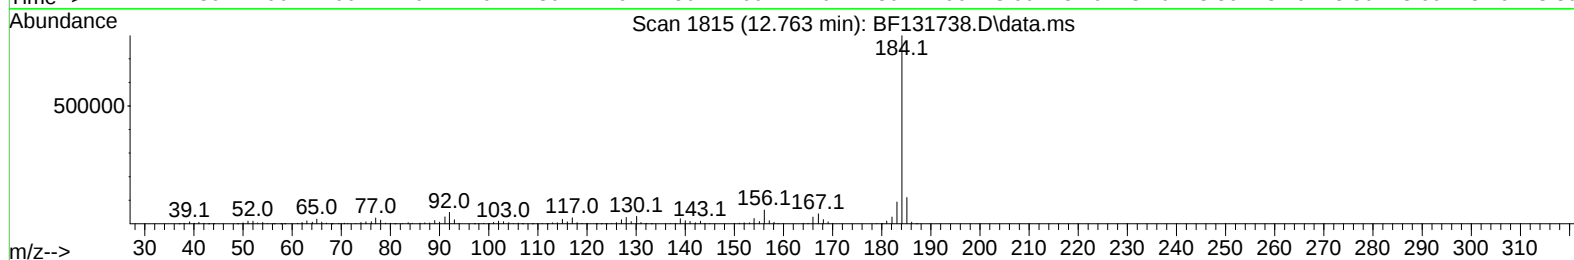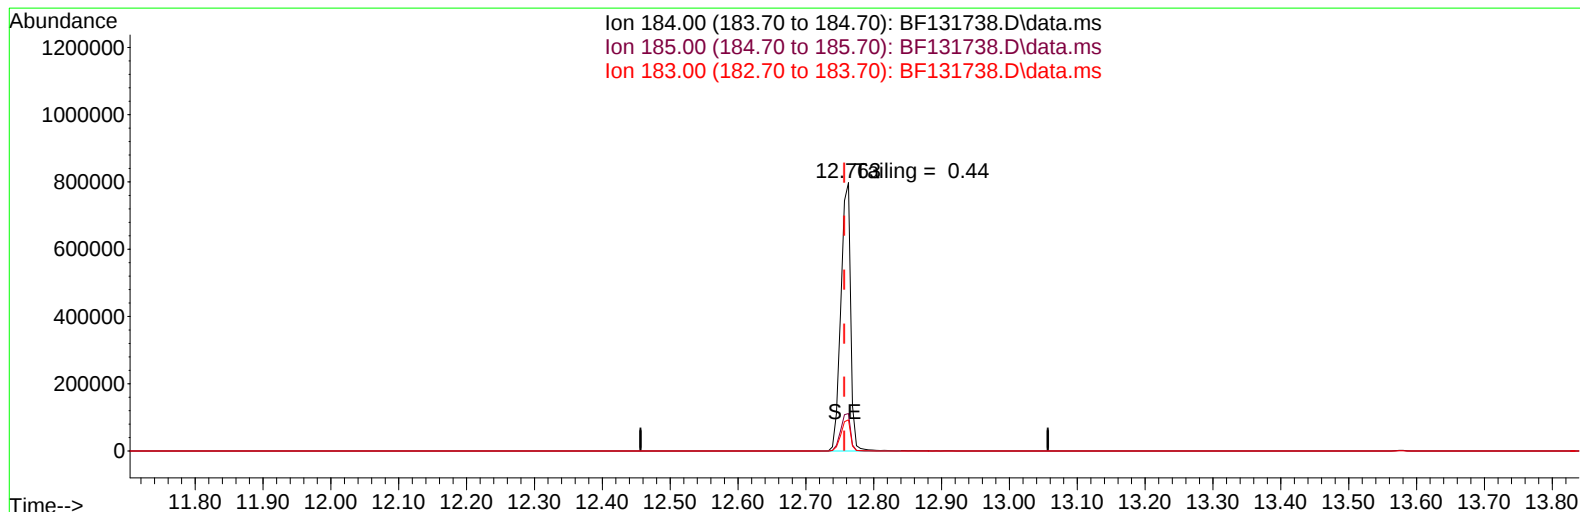

TIC: BF131738.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response **796446**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.99
183.00	11.60	11.63
0.00	0.00	0.00