
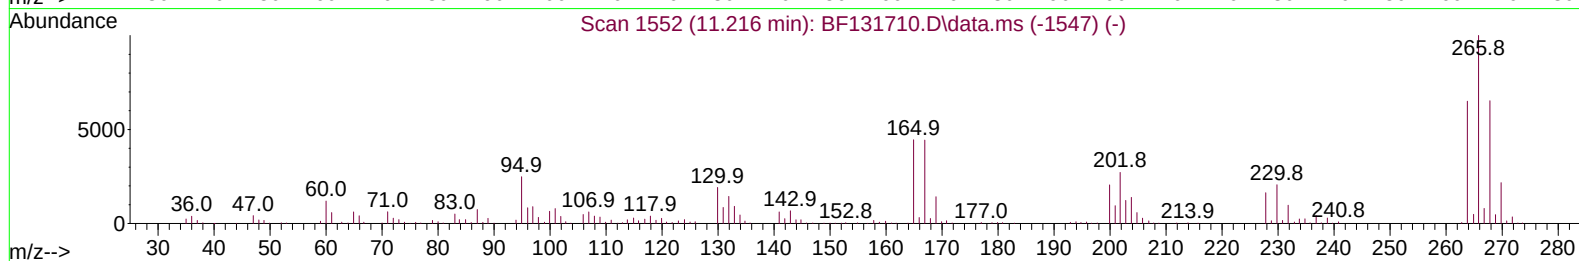
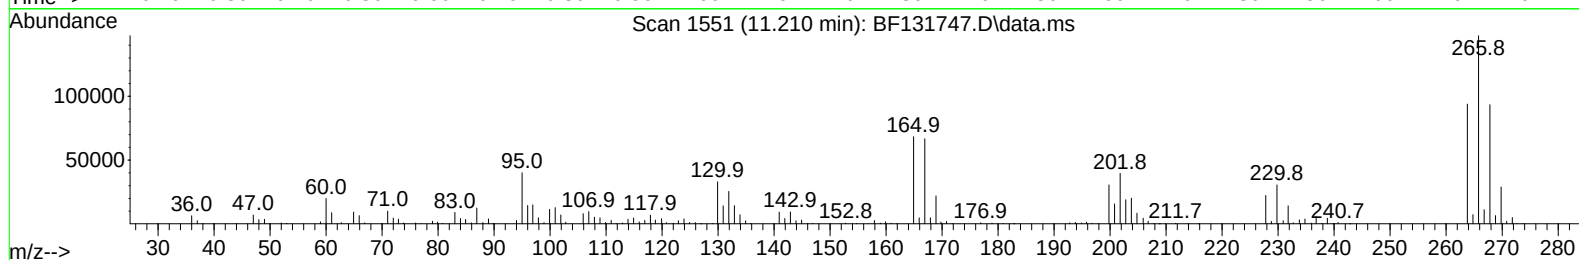


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
Data File : BF131747.D
Acq On : 21 Dec 2022 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 08:18:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

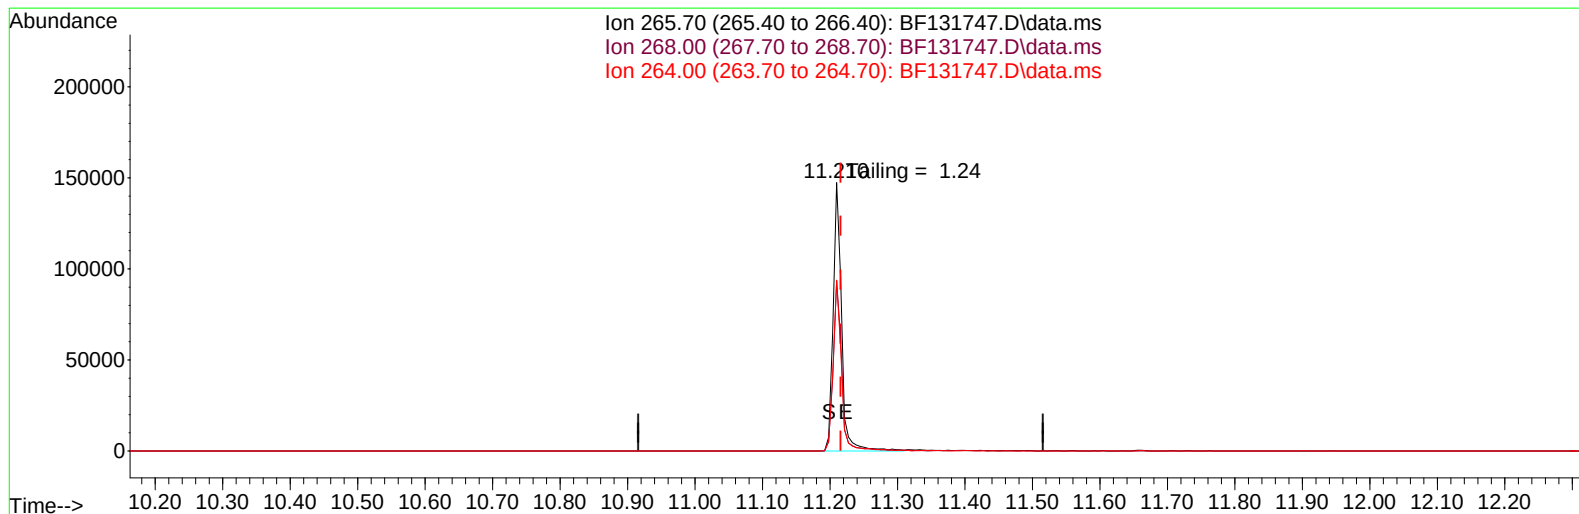

TIC: BF131747.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 30026.70 ng

response 127726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.32
264.00	65.00	63.70
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\  
Data File : BF131747.D  
Acq On    : 21 Dec 2022  15:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 22 08:18:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

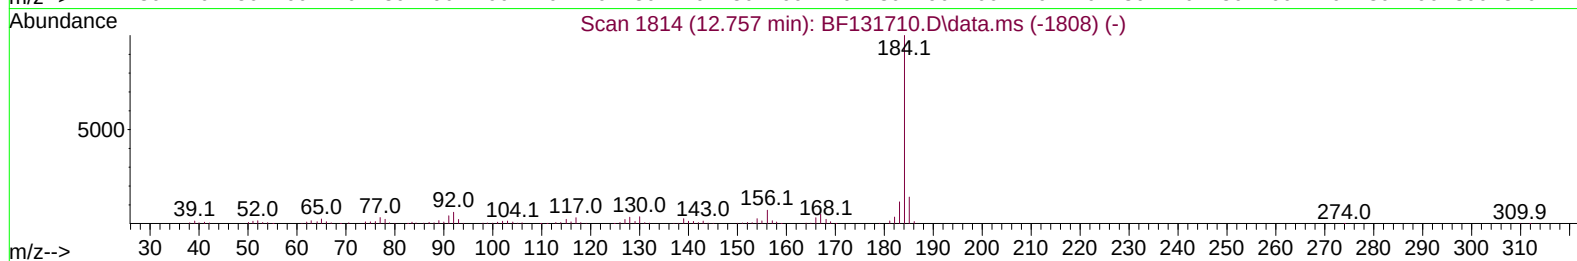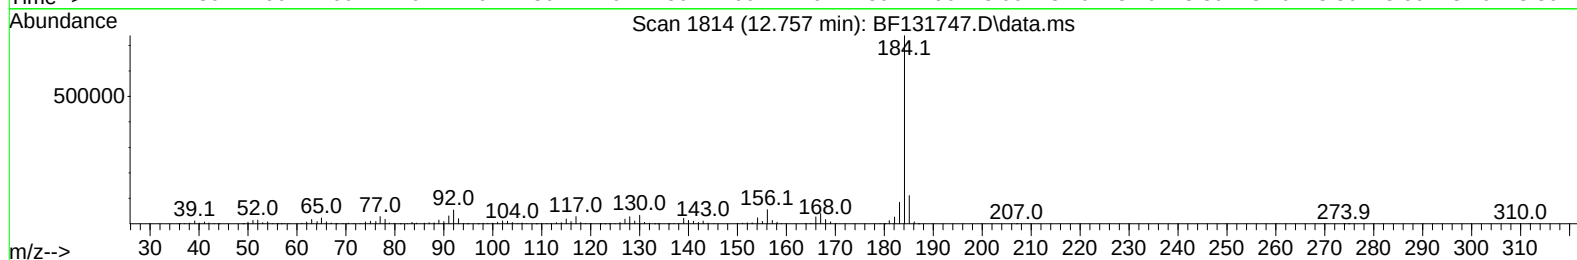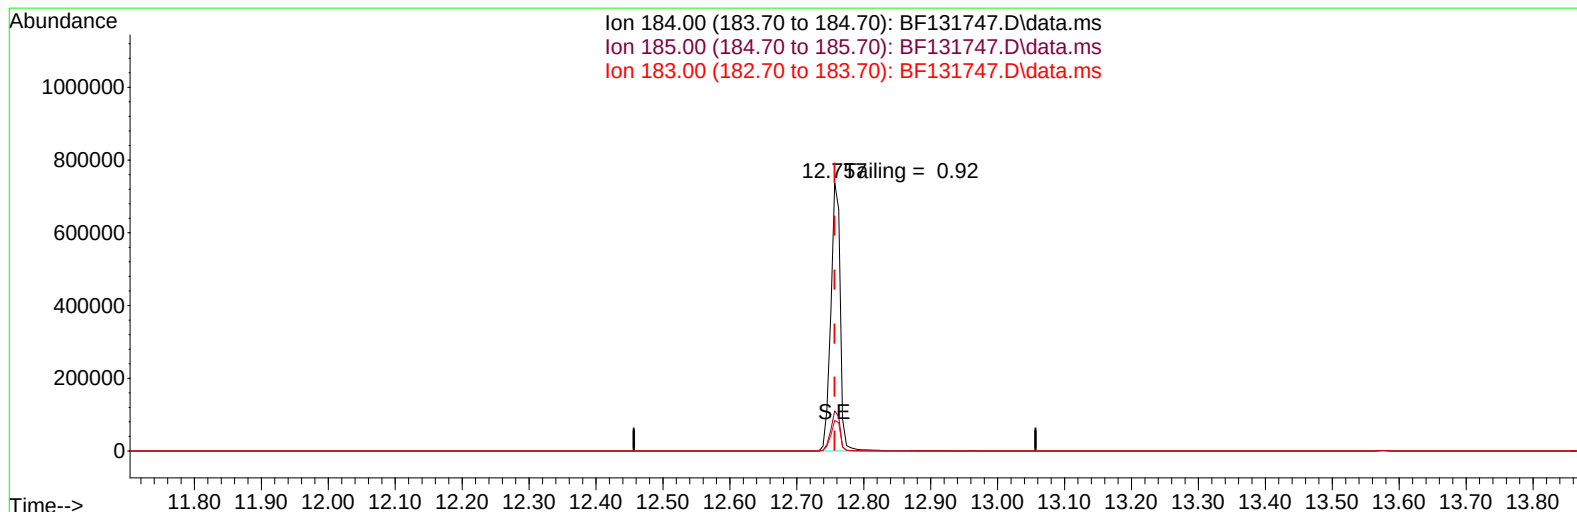

TIC: BF131747.D\data.ms

(77) Benzidine

12.757min (0.000) 0.00 ng

response **725617**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	15.00
183.00	11.60	11.42
0.00	0.00	0.00