
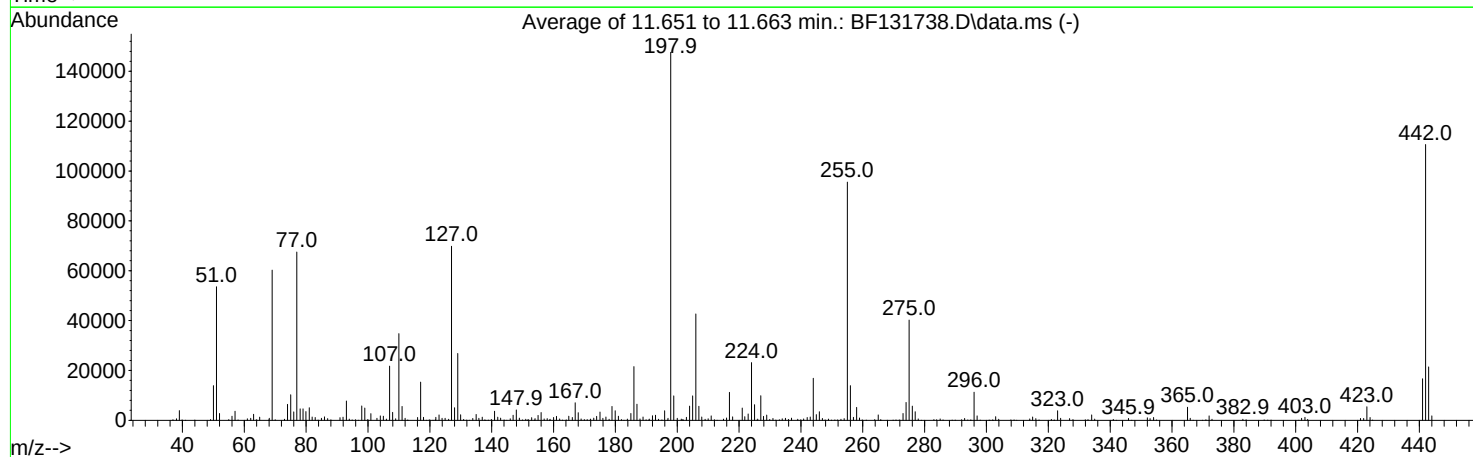


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
 Data File : BF131738.D
 Acq On : 21 Dec 2022 09:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 23 03:03:57 2022

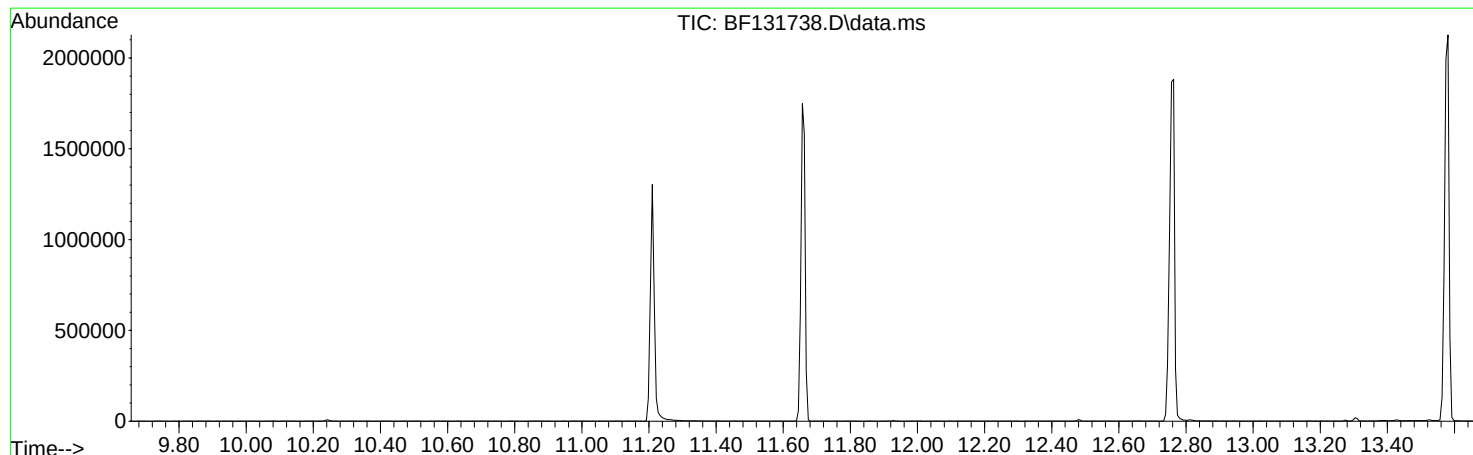




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	53541	PASS
68	69	0.00	2	1.3	777	PASS
69	198	0.00	100	40.8	60243	PASS
70	69	0.00	2	0.4	256	PASS
127	198	10	80	47.3	69792	PASS
197	198	0.00	2	0.6	833	PASS
198	198	100	100	100.0	147571	PASS
199	198	5	9	6.6	9783	PASS
275	198	10	60	27.3	40218	PASS
365	198	1	100	3.5	5220	PASS
441	198	0.01	100	11.3	16647	PASS
442	442	50	100	100.0	110621	PASS
443	442	15	24	19.3	21378	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
 Data File : BF131738.D
 Acq On : 21 Dec 2022 09:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 22 08:12:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 21 03:12:37 2022
 Response via : Initial Calibration

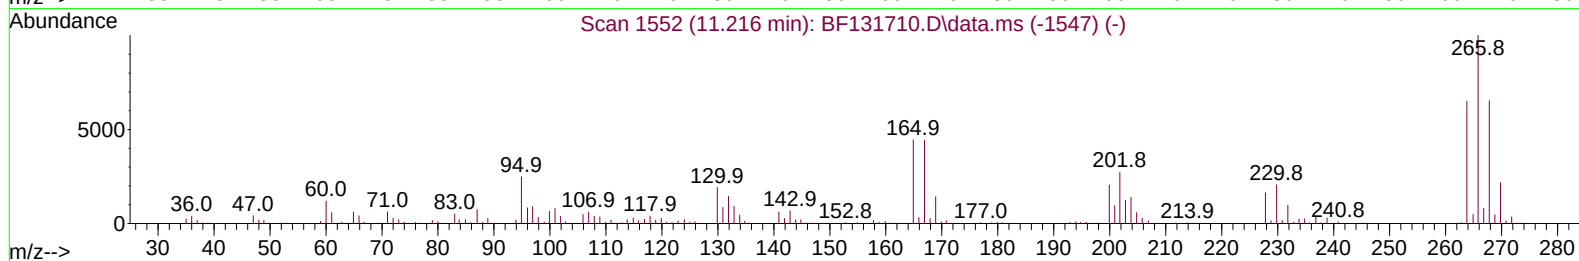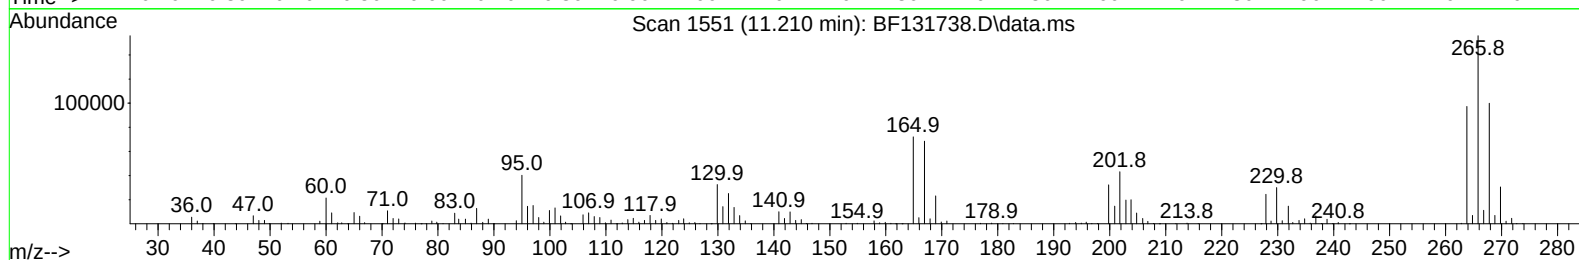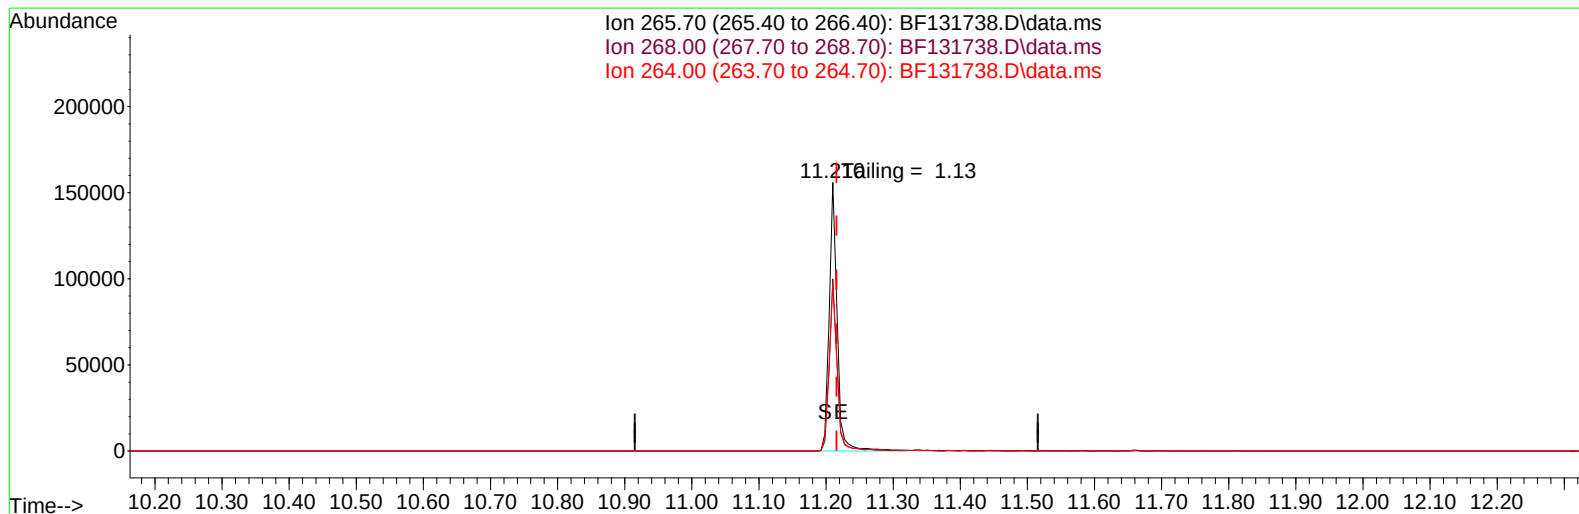

TIC: BF131738.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 30620.82 ng

response 129831

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.10
264.00	65.00	62.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2022	BNA_F	<u>BF131738.D</u>
Compound Name	Response	Retention Time
DDT	393726	13.58
DDD	4296	13.304
DDE	312	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4608	398334	1.16

Instrument :
BNA_F
ClientSampleId :
DFTPP