
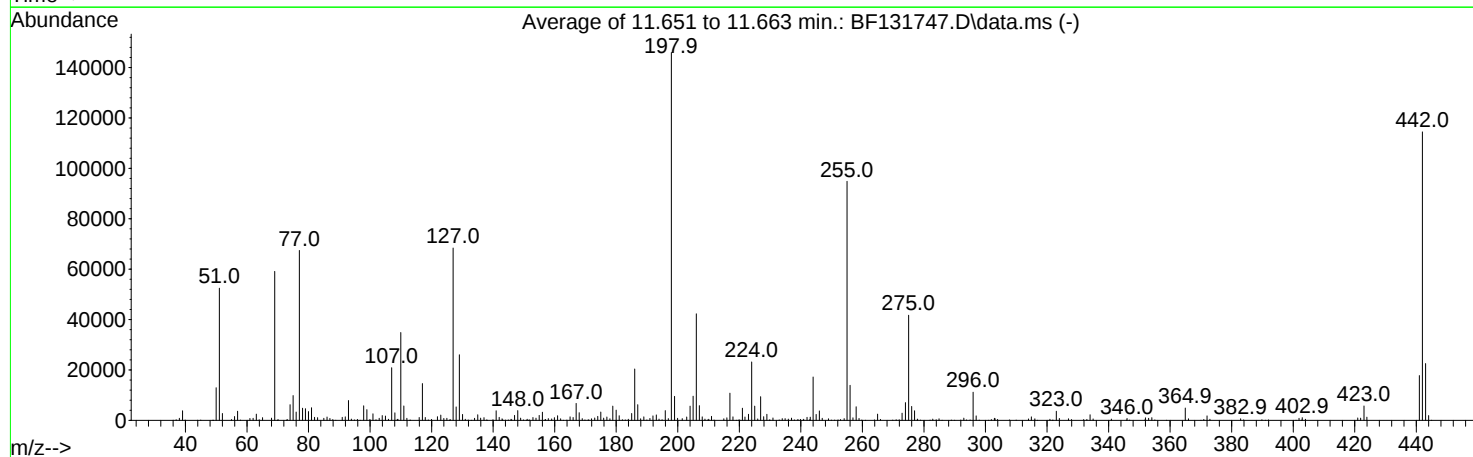


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
 Data File : BF131747.D
 Acq On : 21 Dec 2022 15:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 23 03:03:57 2022

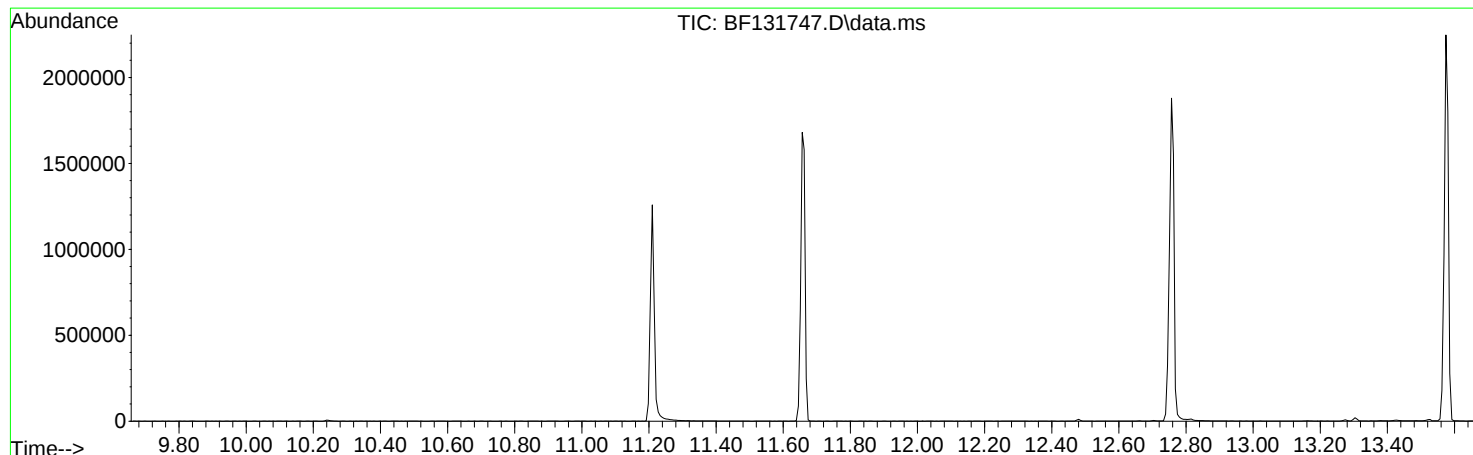




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	52437	PASS
68	69	0.00	2	1.5	894	PASS
69	198	0.00	100	40.5	59061	PASS
70	69	0.00	2	0.4	258	PASS
127	198	10	80	46.8	68347	PASS
197	198	0.00	2	0.5	659	PASS
198	198	100	100	100.0	145981	PASS
199	198	5	9	6.5	9513	PASS
275	198	10	60	28.5	41656	PASS
365	198	1	100	3.3	4883	PASS
441	198	0.01	100	12.2	17782	PASS
442	442	50	100	100.0	114480	PASS
443	442	15	24	19.7	22543	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
Data File : BF131747.D
Acq On : 21 Dec 2022 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 08:18:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

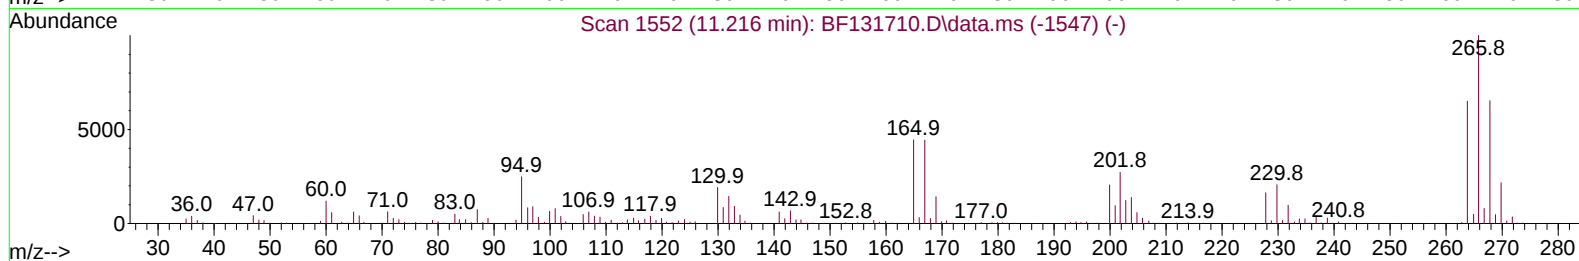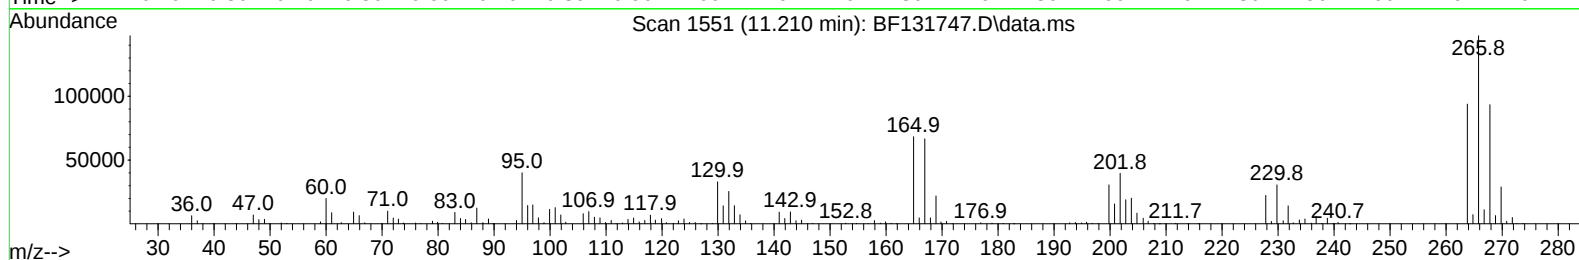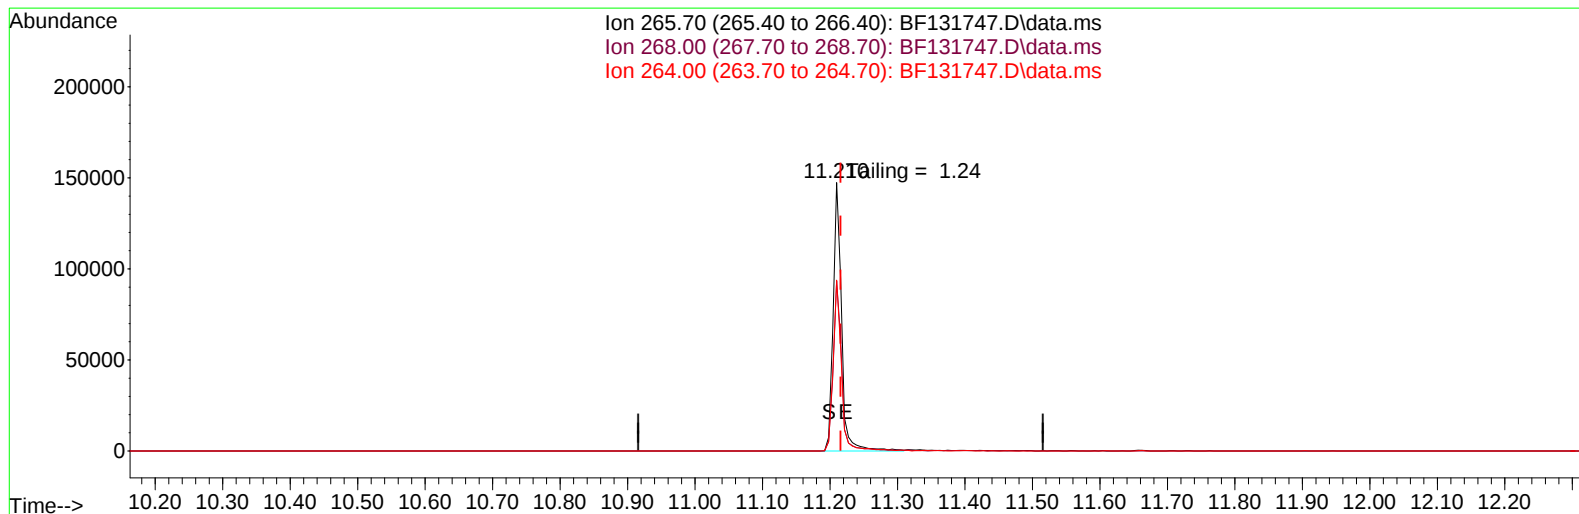

TIC: BF131747.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 30026.70 ng




response 127726

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.32
264.00	65.00	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122122\
Data File : BF131747.D
Acq On : 21 Dec 2022 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 08:18:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 03:12:37 2022
Response via : Initial Calibration

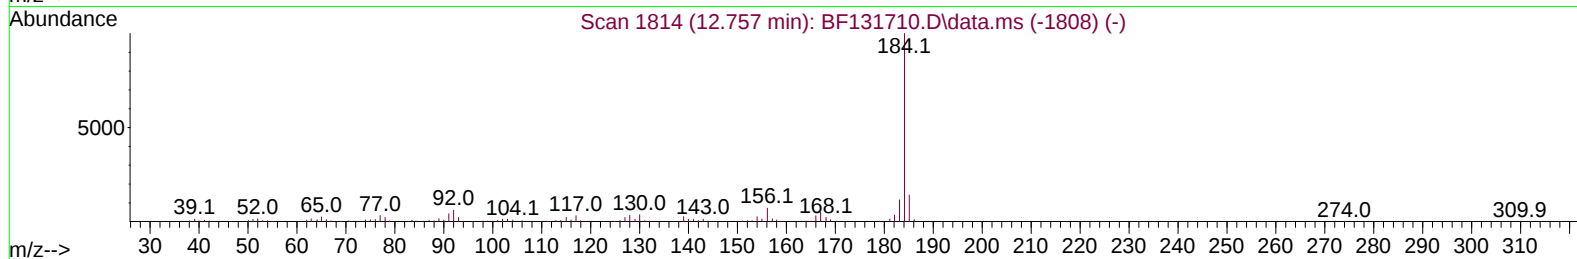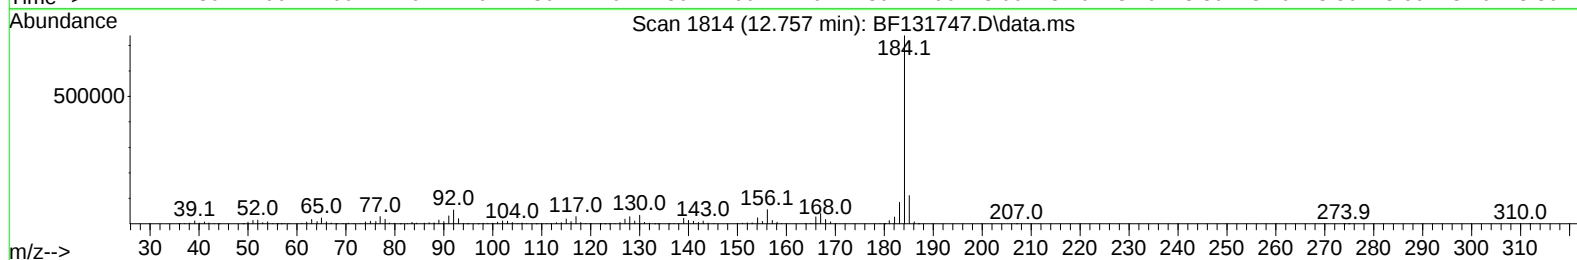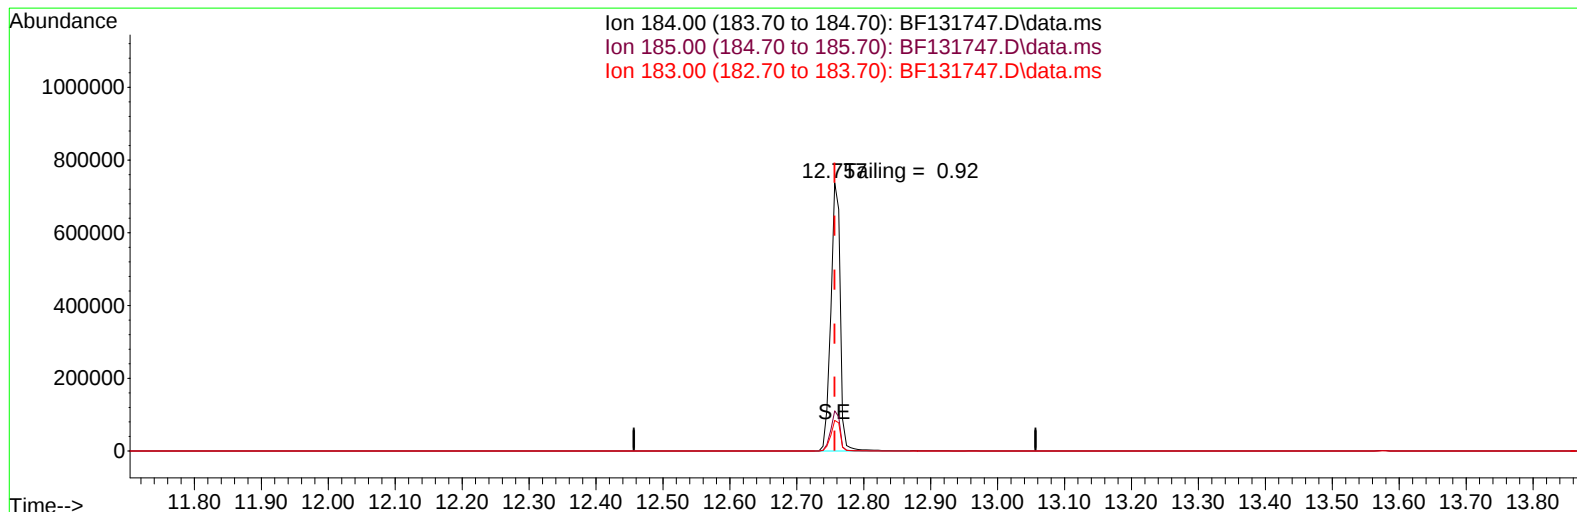

TIC: BF131747.D\data.ms

(77) Benzidine

12.757min (0.000) 0.00 ng

response 725617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	15.00
183.00	11.60	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2022	BNA_F	<u>BF131747.D</u>
Compound Name	Response	Retention Time
DDT	386714	13.574
DDD	5344	13.304
DDE	137	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5481	392195	1.40

Instrument :
BNA_F
ClientSampled :
DFTPP