
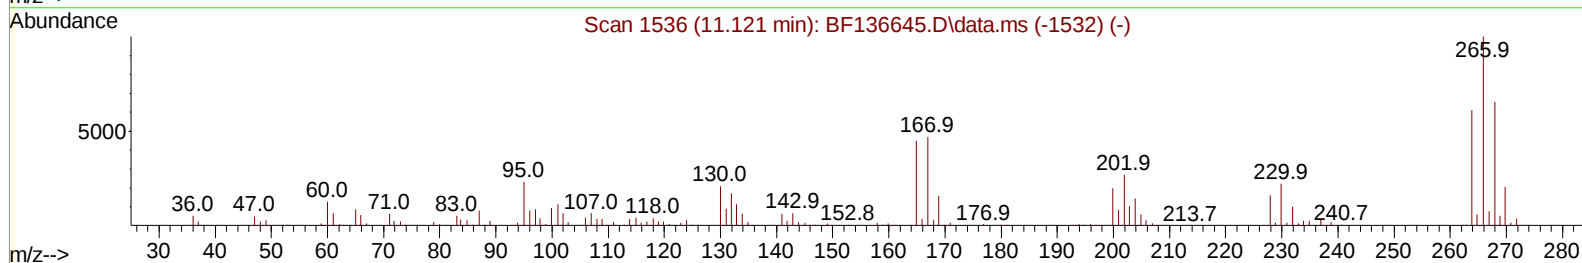
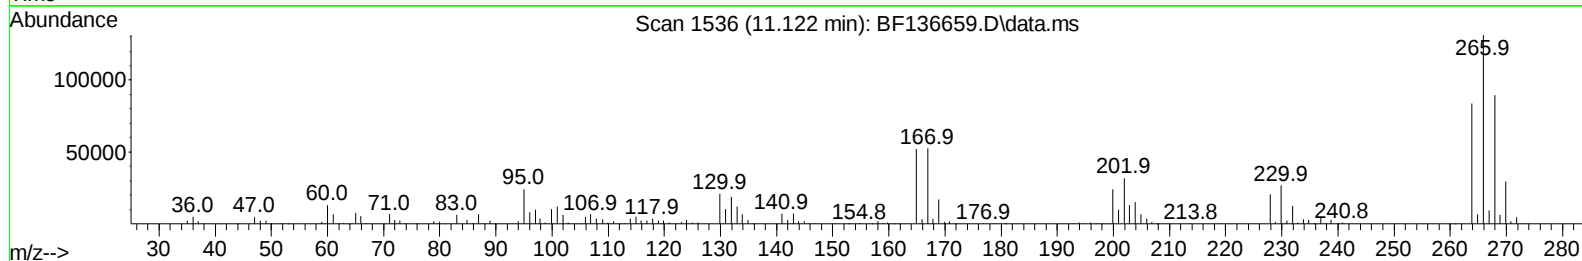


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
Data File : BF136659.D
Acq On : 21 Dec 2023 08:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 23:11:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

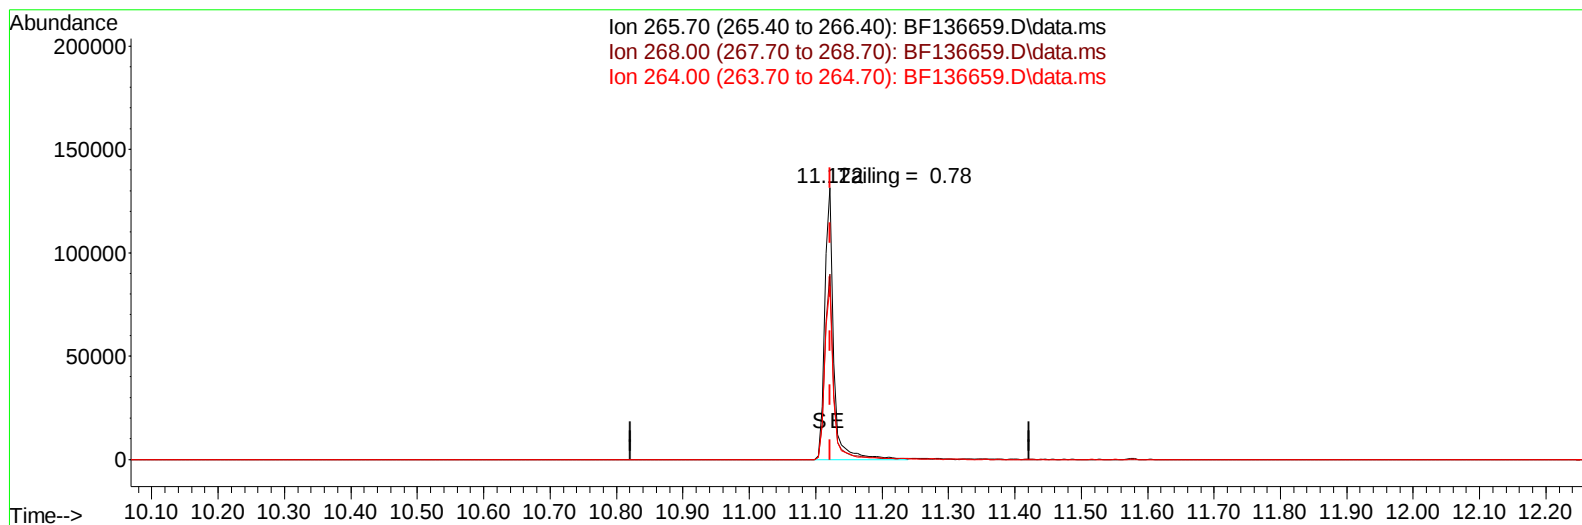




TIC: BF136659.D\data.ms

(70) Pentachlorophenol (C)**11.122min (+ 0.000) 323256.31 ng****response 124941**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	68.24
264.00	61.20	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
Data File : BF136659.D
Acq On : 21 Dec 2023 08:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 23:11:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

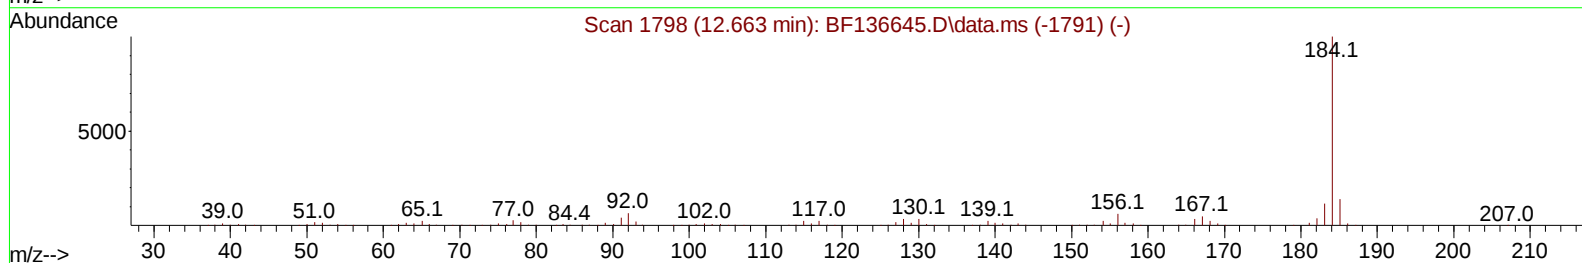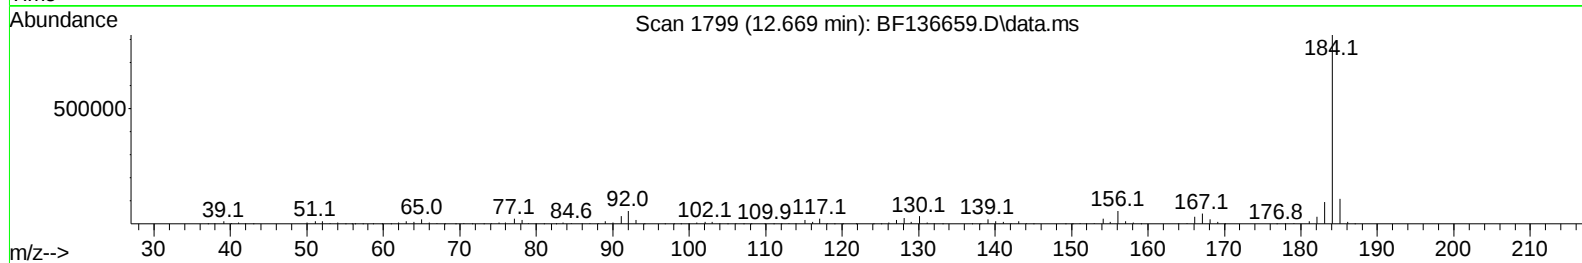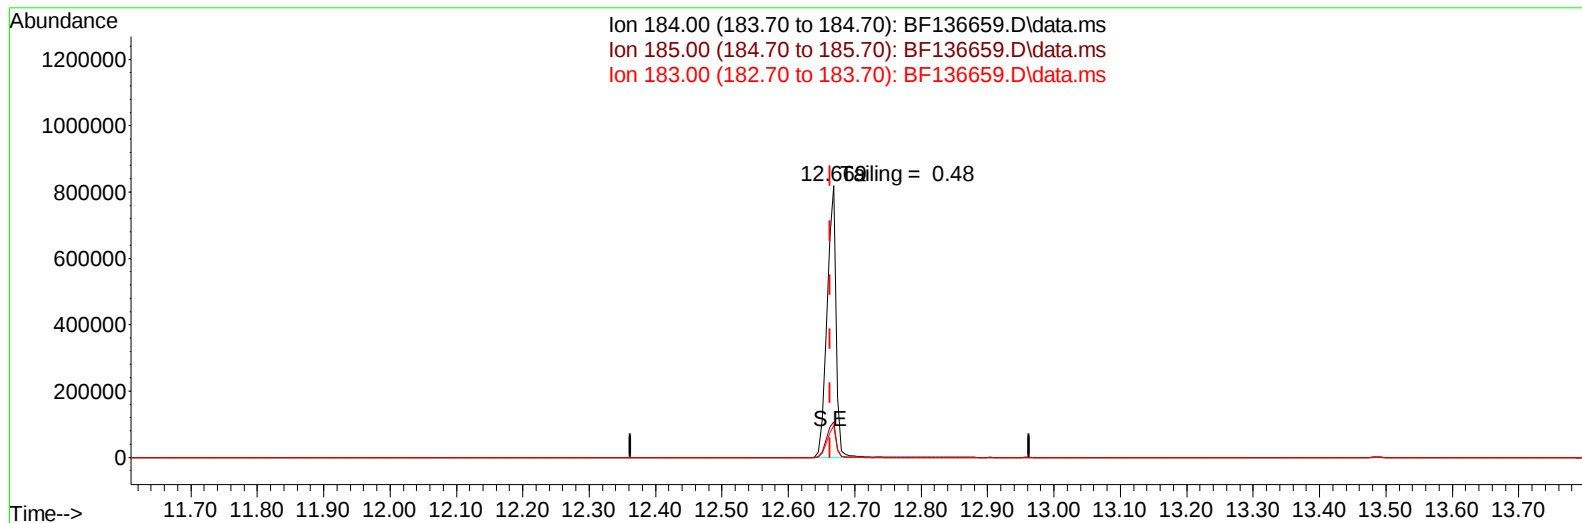

TIC: BF136659.D\data.ms

(77) Benzidine**12.669min (+ 0.006) 0.00 ng****response 783255**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.22
183.00	11.60	11.60
0.00	0.00	0.00