

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
 Data File : BF136667.D
 Acq On : 21 Dec 2023 13:14
 Operator : CG\JU
 Sample : 05585-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P3874-SP4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	562	566	583	rBV	993620	831159	32.67%	6.894%
2	6.416	732	736	749	rBV	618025	503259	19.78%	4.174%
3	6.781	794	798	801	rBV	472570	416772	16.38%	3.457%
4	7.340	888	893	896	rBV	1223143	1347615	52.98%	11.178%
5	8.057	1010	1015	1018	rBV	616545	542406	21.32%	4.499%
6	9.134	1193	1198	1201	rBV	2585241	2543823	100.00%	21.101%
7	9.810	1309	1313	1317	rBV	742529	609548	23.96%	5.056%
8	10.604	1444	1448	1466	rBV	1452628	1421994	55.90%	11.795%
9	11.304	1563	1567	1570	rBV	751159	632001	24.84%	5.242%
10	11.839	1655	1658	1667	rBV	54466	62782	2.47%	0.521%
11	12.627	1789	1792	1800	rBV2	22128	28940	1.14%	0.240%
12	12.904	1834	1839	1842	rBV	2559136	2317640	91.11%	19.224%
13	13.951	2013	2017	2025	rBV	436471	417078	16.40%	3.460%
14	15.427	2263	2268	2273	rBV	303320	380659	14.96%	3.158%




Sum of corrected areas: 12055676

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
Data File : BF136667.D
Acq On : 21 Dec 2023 13:14
Operator : CG\JU
Sample : 05585-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P3874-SP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

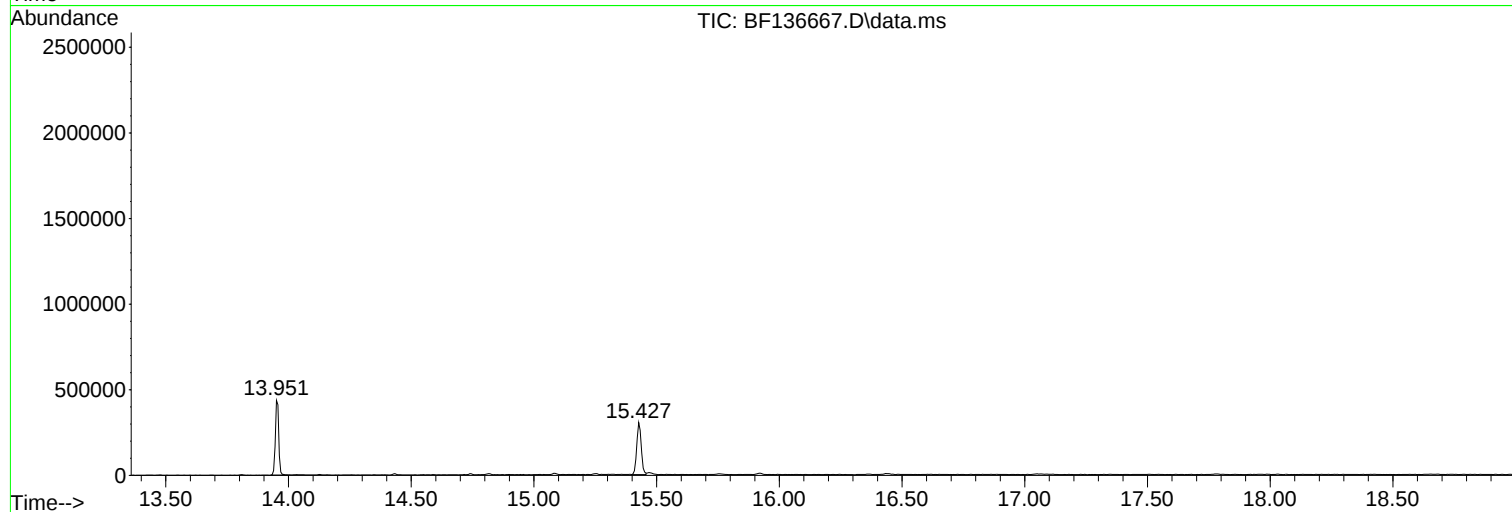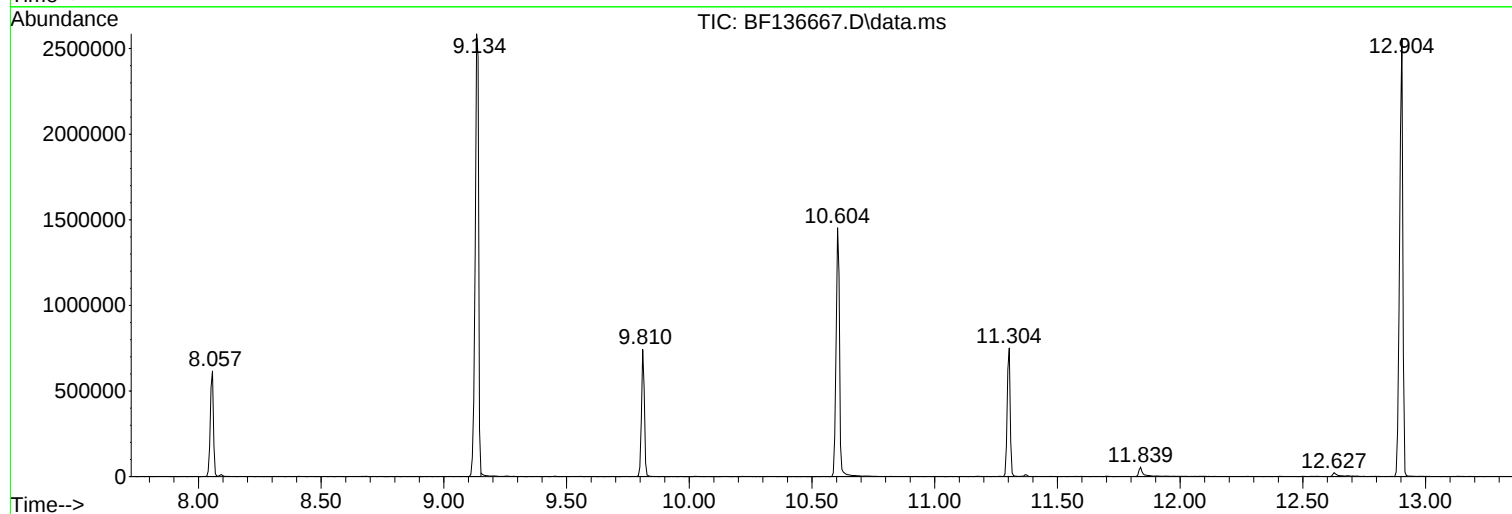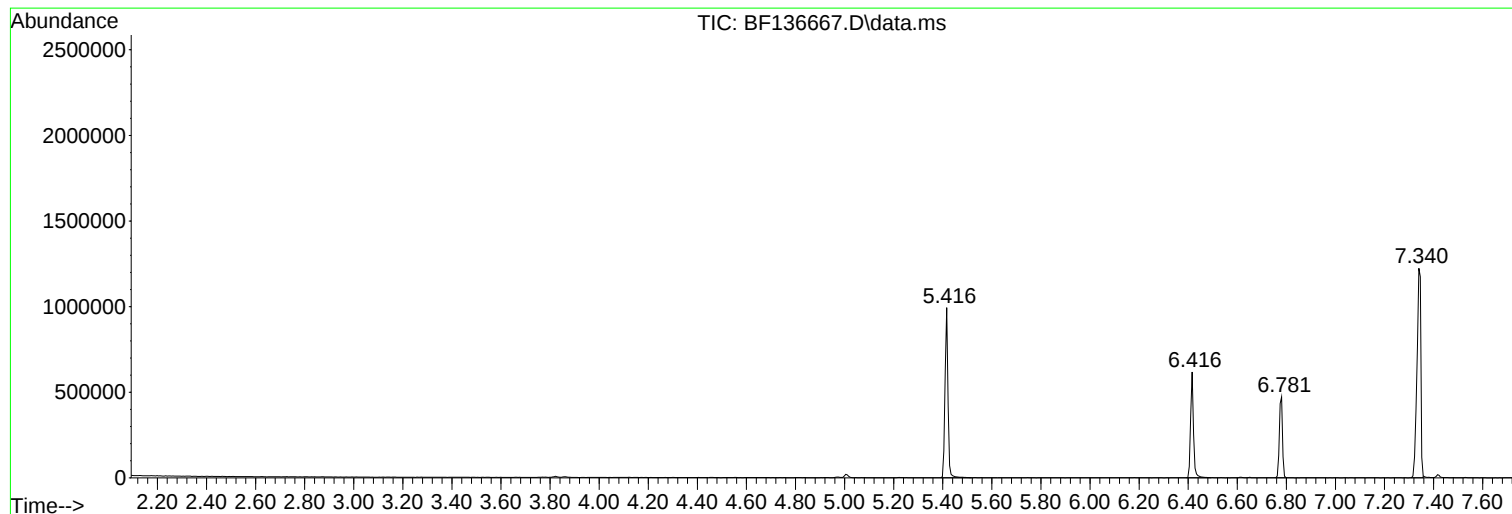

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
Data File : BF136667.D
Acq On : 21 Dec 2023 13:14
Operator : CG\JU
Sample : 05585-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P3874-SP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
Data File : BF136667.D
Acq On : 21 Dec 2023 13:14
Operator : CG\JU
Sample : 05585-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P3874-SP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------