
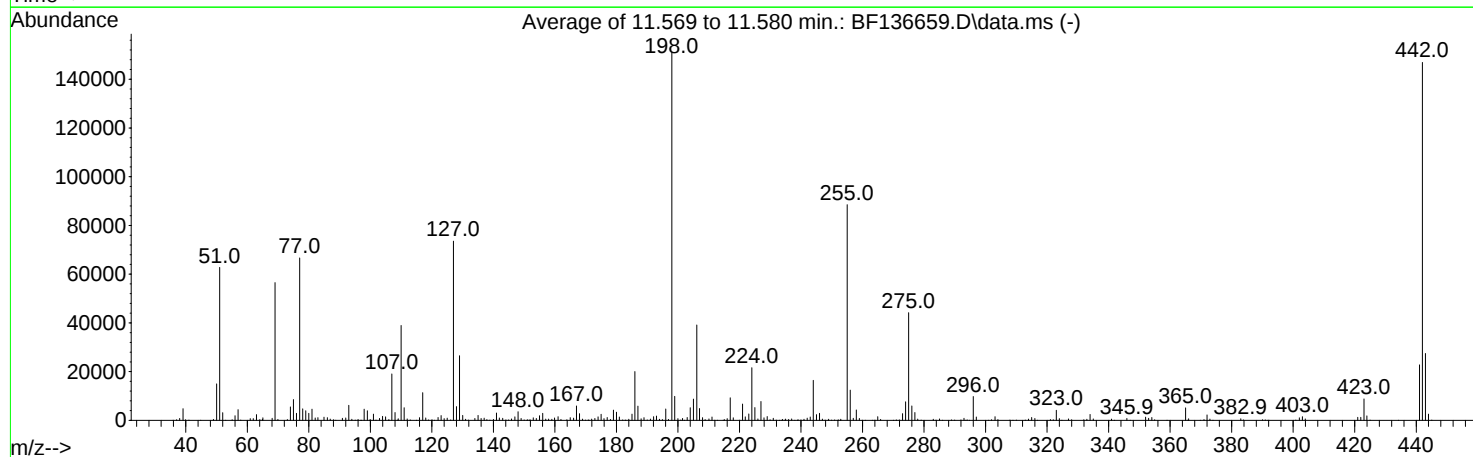


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
 Data File : BF136659.D
 Acq On : 21 Dec 2023 08:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 21 01:54:25 2023

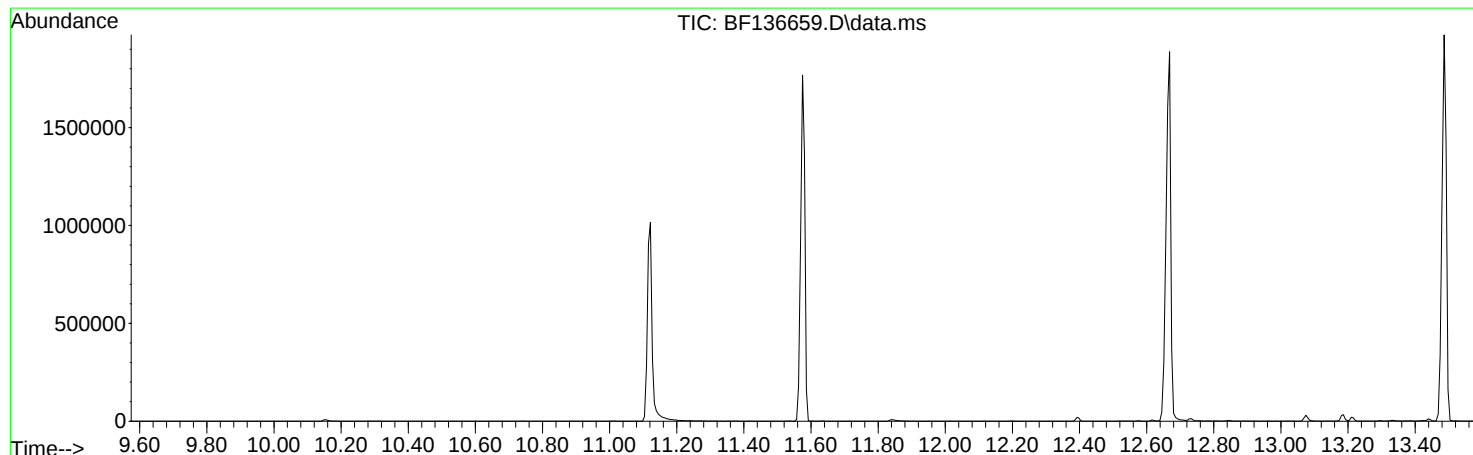




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	62781	PASS
68	69	0.00	2	1.5	839	PASS
69	198	0.00	100	37.4	56512	PASS
70	69	0.00	2	0.7	370	PASS
127	198	10	80	48.7	73536	PASS
197	198	0.00	2	0.3	391	PASS
198	198	100	100	100.0	150976	PASS
199	198	5	9	6.5	9863	PASS
275	198	10	60	29.3	44189	PASS
365	198	1	100	3.4	5144	PASS
441	198	0.01	100	15.1	22769	PASS
442	442	50	100	100.0	146915	PASS
443	442	15	24	18.7	27470	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122123\
Data File : BF136659.D
Acq On : 21 Dec 2023 08:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 21 23:11:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

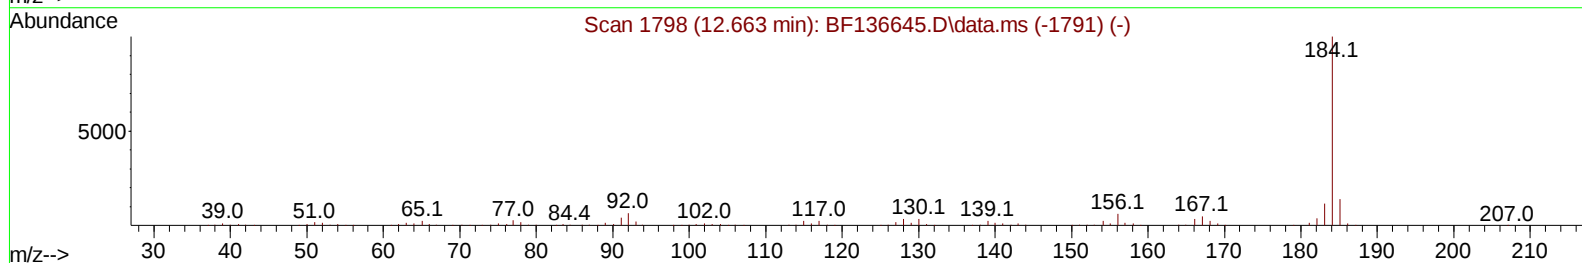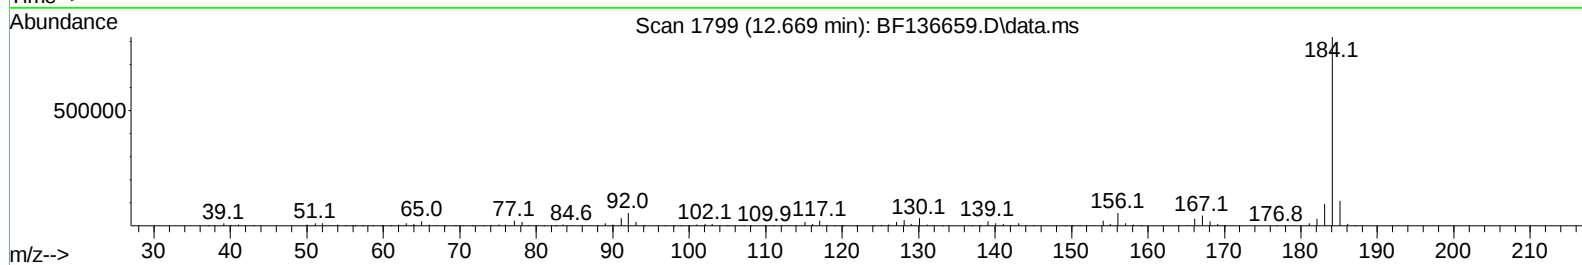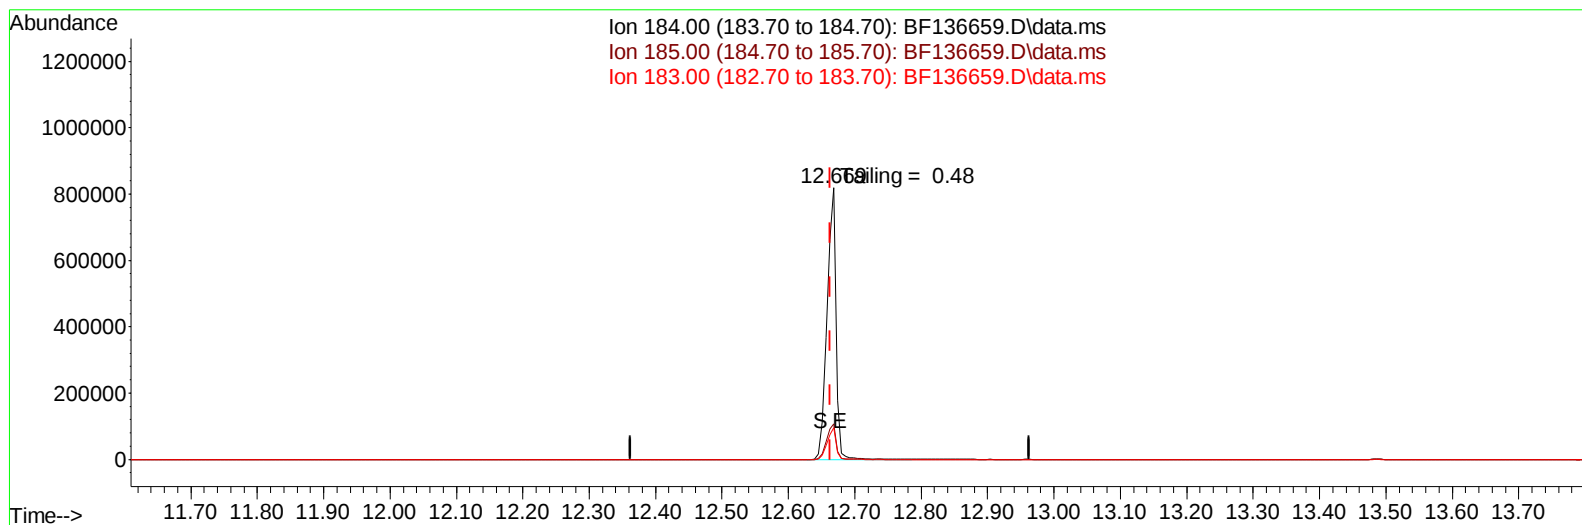

TIC: BF136659.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng

response 783255

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.22
183.00	11.60	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2023	BNA_F	<u>BF136659.D</u>
Compound Name	Response	Retention Time
DDT	375706	13.496
DDD	10491	13.186
DDE	784	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11275	386981	2.91

Instrument :
BNA_F
ClientSampleId :
DFTPP