

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122215\
 Data File : BF084013.D
 Acq On : 23 Dec 2015 2:53
 Operator : UM/SJ
 Sample : G4916-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20151214MGP209BRV46.5

Quant Time: Dec 23 03:17:42 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 22 18:54:09 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	43141	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	174305	20.00	ng	0.00
38) Acenaphthene-d10	9.87	164	83911	20.00	ng	0.00
63) Phenanthrene-d10	11.36	188	163002	20.00	ng	0.00
75) Chrysene-d12	13.99	240	168155	20.00	ng	-0.01
86) Perylene-d12	15.41	264	142464	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	182635	72.18	ng	0.01
7) Phenol-d6	6.48	99	138030	46.40	ng	0.00
23) Nitrobenzene-d5	7.39	82	254870	89.83	ng	0.00
41) 2,4,6-Tribromophenol	10.66	330	140276	173.80	ng	0.00
44) 2-Fluorobiphenyl	9.20	172	634216	101.72	ng	0.00
78) Terphenyl-d14	12.93	244	656737	93.14	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.60	77	8152	4.10	ng	90
15) Benzyl Alcohol	6.98	79	4697	2.01	ng	# 46
19) n-Nitroso-di-n-propylamine	7.39	70	36119	20.04	ng	# 78
25) Isophorone	7.39	82	223563	41.58	ng	# 66
50) 2,6-Dinitrotoluene	9.87	165	10487	7.57	ng	# 35
56) 2,4-Dinitrotoluene	9.87	165	10487	6.02	ng	# 20
66) 4-Bromophenyl-phenylether	10.66	248	10181	5.45	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122215\
Data File : BF084013.D
Acq On : 23 Dec 2015 2:53
Operator : UM/SJ
Sample : G4916-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20151214MGP209BRV46.5

Quant Time: Dec 23 03:17:42 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 18:54:09 2015
Response via : Initial Calibration

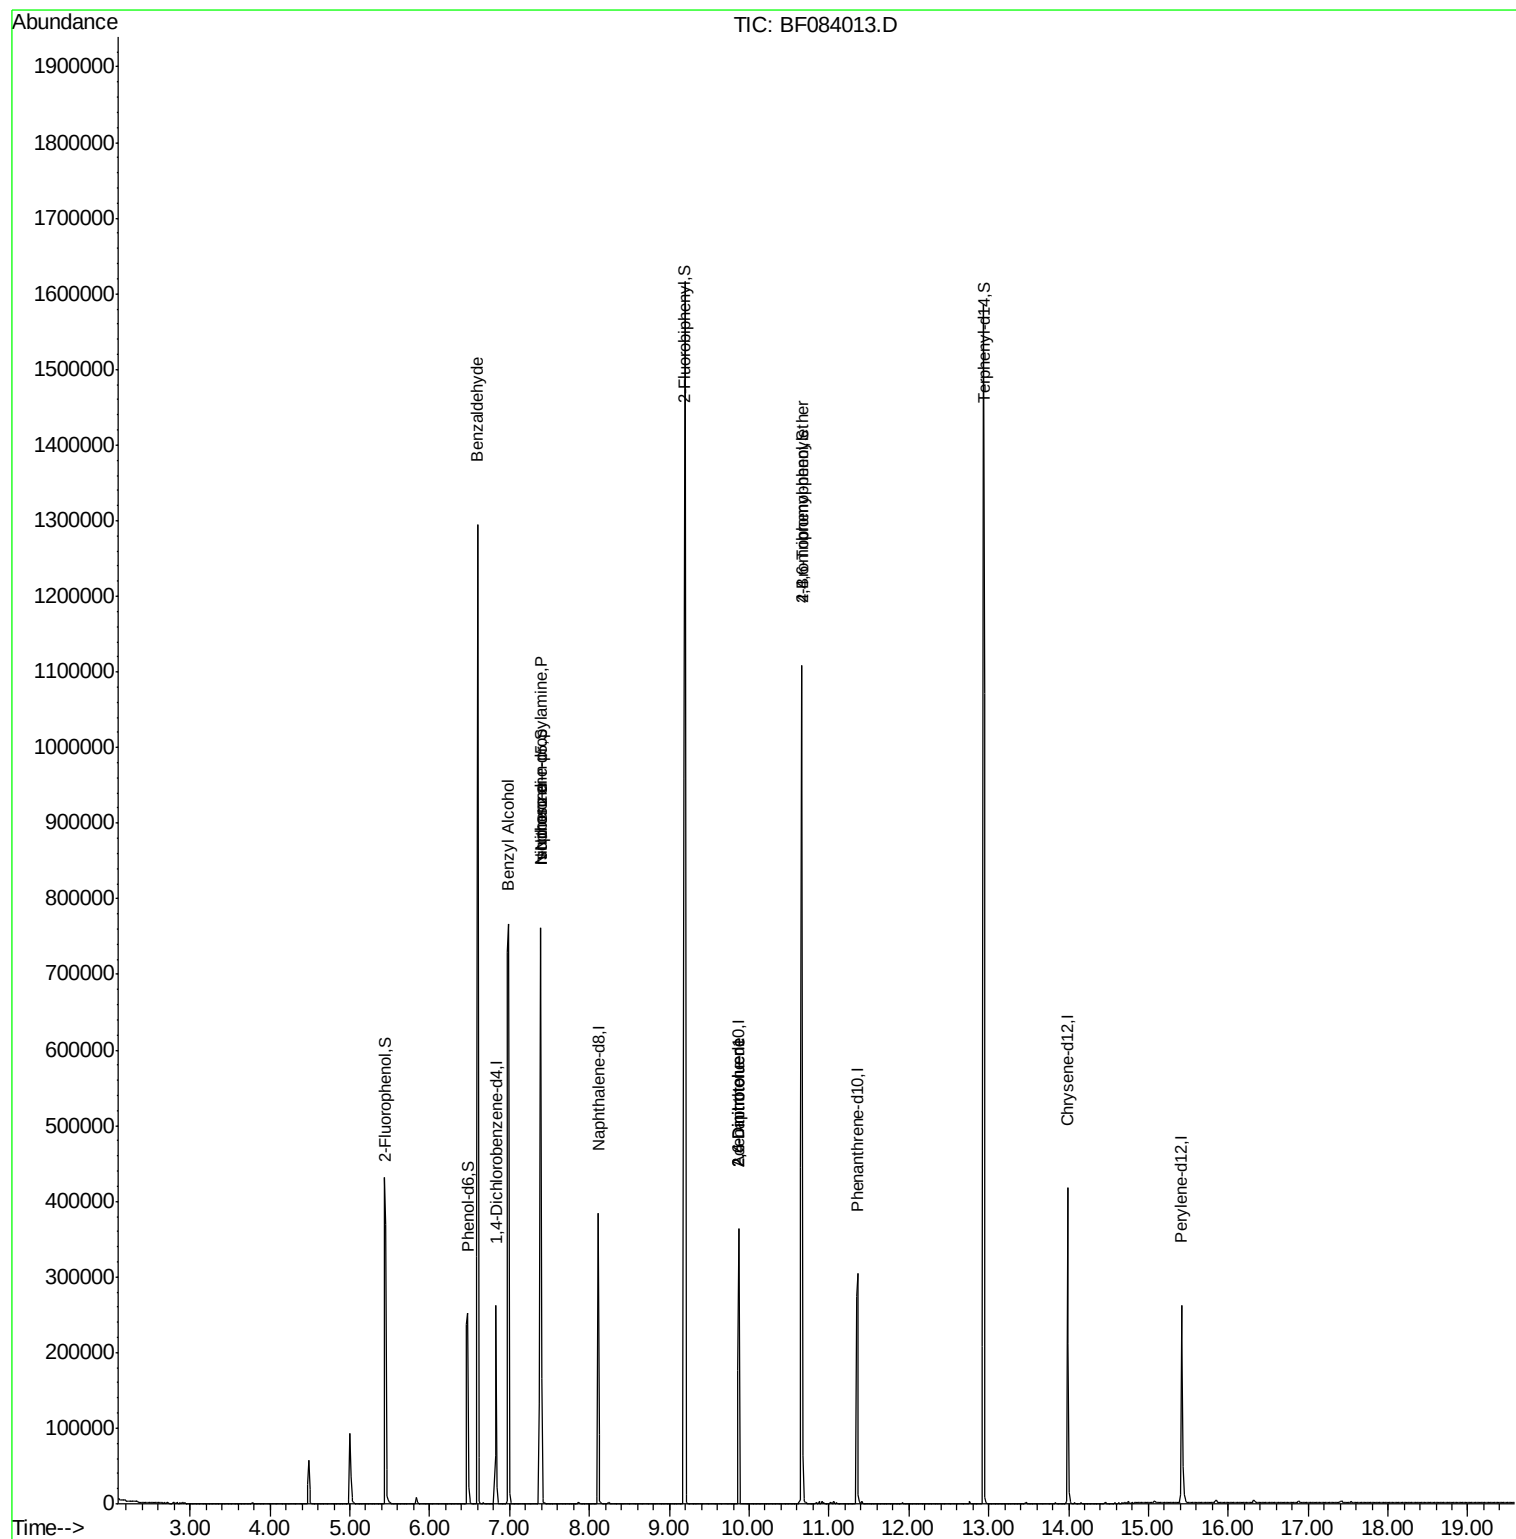


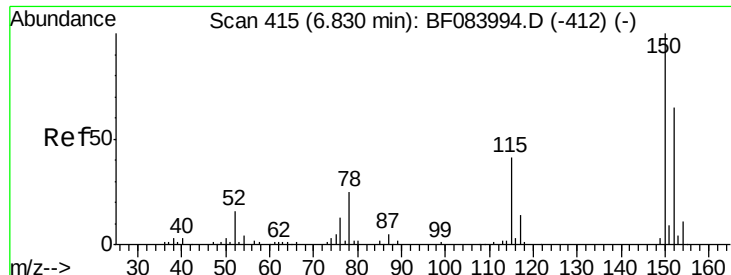




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.83 min Scan# 415
 Delta R.T. -0.00 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Instrument :
 BNA_F
 ClientSampleId :
 20151214MGP209BRV46.5

Tgt Ion:152 Resp: 43141
 Ion Ratio Lower Upper
 152 100
 150 151.3 123.0 184.4
 115 59.2 51.4 77.2

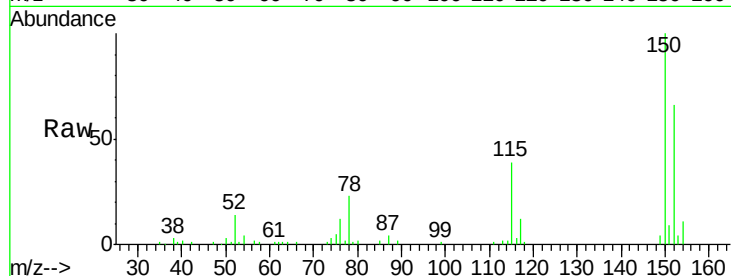


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E


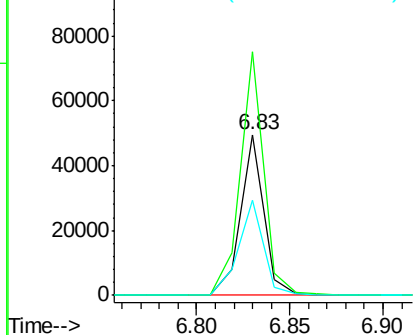



#5
 2-Fluorophenol
 Concen: 72.18 ng
 RT: 5.45 min Scan# 294
 Delta R.T. 0.01 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Tgt Ion:112 Resp: 182635
 Ion Ratio Lower Upper
 112 100
 64 43.5 36.6 55.0
 63 24.0 19.4 29.0



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

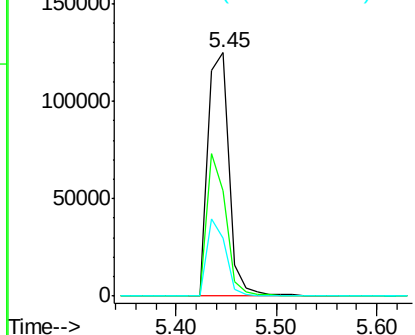

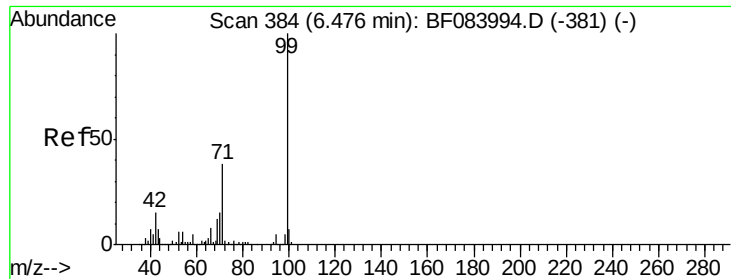

#7

Phenol-d6

Concen: 46.40 ng

RT: 6.48 min Scan# 384

Delta R.T. -0.00 min

Lab File: BF084013.D

Acq: 23 Dec 2015 2:53

Instrument :

BNA_F

ClientSampleId :

20151214MGP209BRV46.5


Tgt Ion: 99 Resp: 138030

Ion Ratio Lower Upper

99 100

42 11.9 12.8 19.2#




71 31.9 30.9 46.3

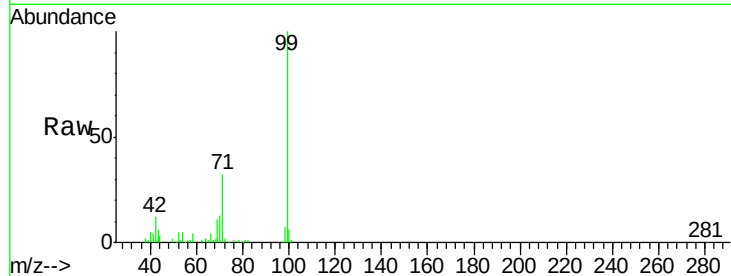

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

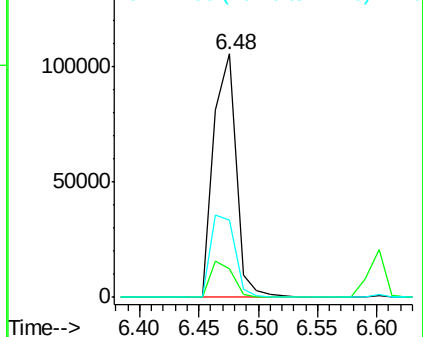

#9

Benzaldehyde

Concen: 4.10 ng

RT: 6.60 min Scan# 395

Delta R.T. 0.23 min

Lab File: BF084013.D

Acq: 23 Dec 2015 2:53


Tgt Ion: 77 Resp: 8152

Ion Ratio Lower Upper

77 100

105 85.2 83.0 123.0



106 92.9 74.6 114.6




Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E




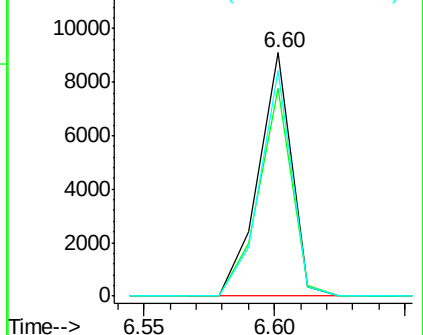




#15
Benzyl Alcohol
Concen: 2.01 ng
RT: 6.98 min Scan# 428
Delta R.T. -0.00 min
Lab File: BF084013.D
Acq: 23 Dec 2015 2:53




Instrument :
BNA_F
ClientSampleId :
20151214MGP209BRV46.5


Tgt Ion: 79 Resp: 4697
Ion Ratio Lower Upper
79 100
108 28.4 69.0 103.4#
77 94.5 50.0 75.0#

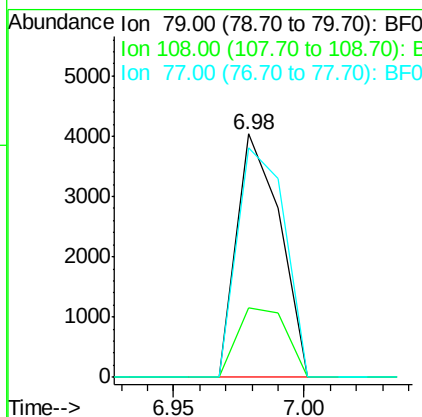

#19
n-Nitroso-di-n-propylamine
Concen: 20.04 ng
RT: 7.39 min Scan# 464
Delta R.T. 0.15 min
Lab File: BF084013.D
Acq: 23 Dec 2015 2:53

Tgt Ion: 70 Resp: 36119
Ion Ratio Lower Upper
70 100
42 41.5 33.3 49.9
101 0.0 9.3 13.9#
130 2.3 23.4 35.0#

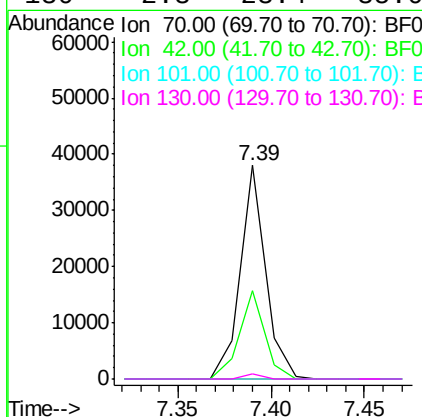







#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.11 min Scan# 527
Delta R.T. -0.00 min
Lab File: BF084013.D
Acq: 23 Dec 2015 2:53

Instrument :
BNA_F
ClientSampleId :
20151214MGP209BRV46.5

Tgt Ion:	136	Resp:	174305
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.7	13.1
54	6.7	5.8	8.8
68	4.7	4.2	6.2

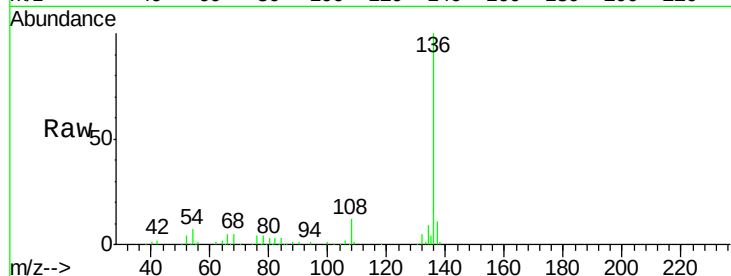


Abundance Ion 136.00 (135.70 to 136.70): E
300000
Ion 137.00 (136.70 to 137.70): E
250000
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

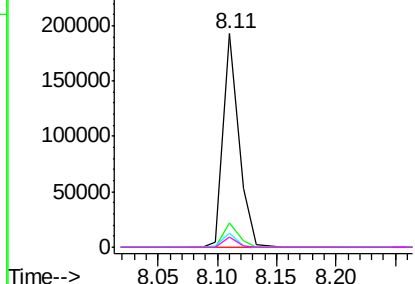




#23
Nitrobenzene-d5
Concen: 89.83 ng
RT: 7.39 min Scan# 464
Delta R.T. -0.00 min
Lab File: BF084013.D
Acq: 23 Dec 2015 2:53

Tgt Ion:	82	Resp:	254870
Ion	Ratio	Lower	Upper
82	100		
128	43.9	34.6	51.8
54	48.4	38.4	57.6



Abundance Ion 82.00 (81.70 to 82.70): BF0
300000
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

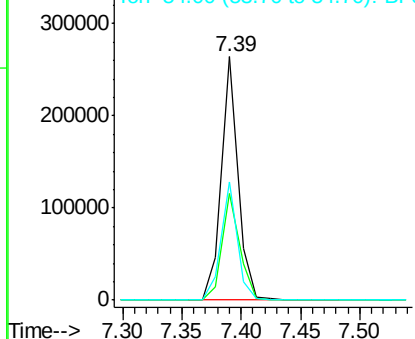



#25

Isophorone

Concen: 41.58 ng

RT: 7.39 min Scan# 464

Delta R.T. -0.26 min

Lab File: BF084013.D

Acq: 23 Dec 2015 2:53

Instrument :

BNA_F

ClientSampleId :

20151214MGP209BRV46.5


Tgt Ion: 82 Resp: 223563

Ion Ratio Lower Upper

82 100

95 0.0 6.6 10.0#




138 0.0 13.6 20.4#

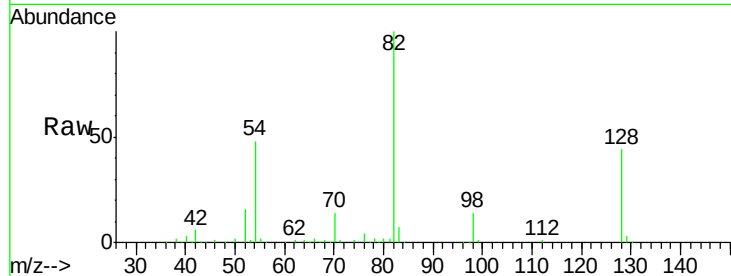

Abundance Ion 82.00 (81.70 to 82.70): BF084013.D (-461) (-)

Ion 95.00 (94.70 to 95.70): BF084013.D (-461) (-)

Ion 138.00 (137.70 to 138.70): BF084013.D (-461) (-)

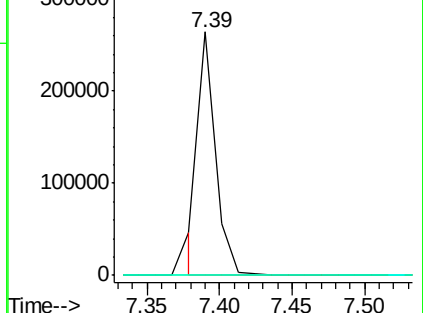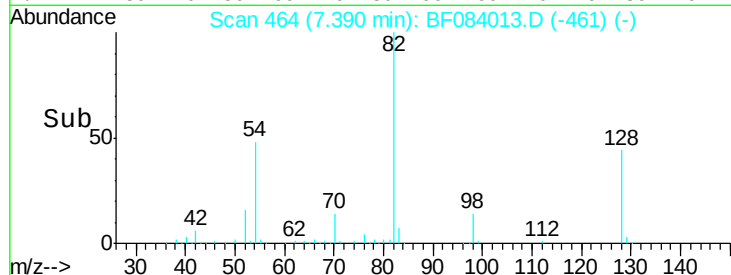

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.87 min Scan# 681

Delta R.T. -0.00 min

Lab File: BF084013.D

Acq: 23 Dec 2015 2:53


Tgt Ion: 164 Resp: 83911

Ion Ratio Lower Upper

164 100

162 103.0 85.1 127.7



160 47.0 37.5 56.3




Abundance Ion 164.00 (163.70 to 164.70): BF084013.D (-655) (-)

Ion 162.00 (161.70 to 162.70): BF084013.D (-655) (-)

Ion 160.00 (159.70 to 160.70): BF084013.D (-655) (-)

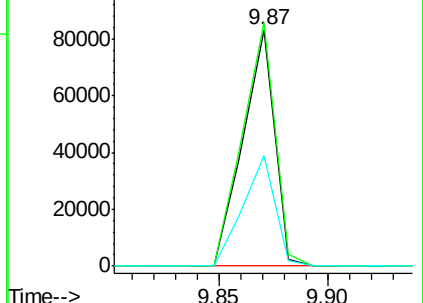


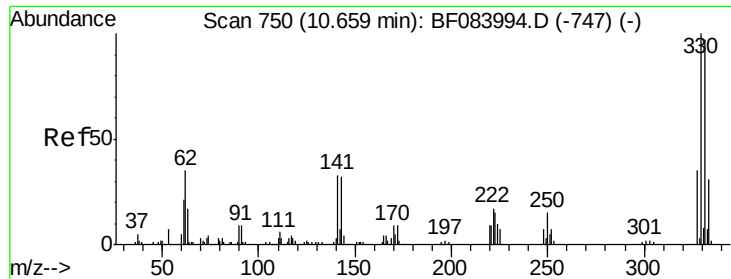




#41
 2,4,6-Tribromophenol
 Concen: 173.80 ng
 RT: 10.66 min Scan# 750
 Delta R.T. -0.00 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Instrument :
 BNA_F
 ClientSampleId :
 20151214MGP209BRV46.5

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.4	76.6	114.8
141	41.0	27.8	41.6




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

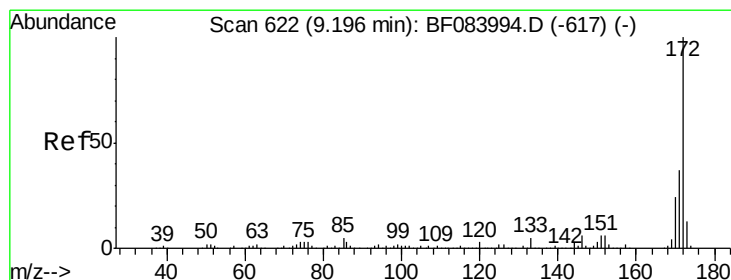
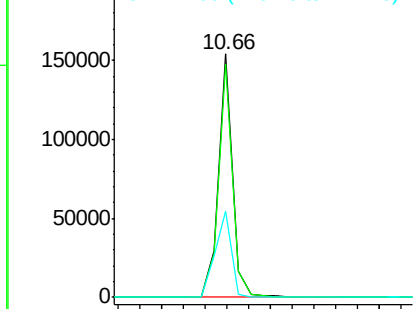



#44
 2-Fluorobiphenyl
 Concen: 101.72 ng
 RT: 9.20 min Scan# 622
 Delta R.T. 0.00 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.9	43.3
170	23.9	18.6	27.8

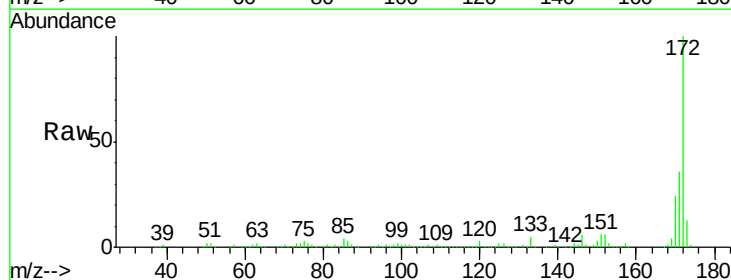

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



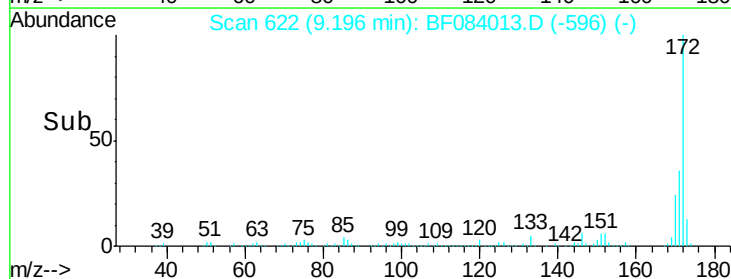
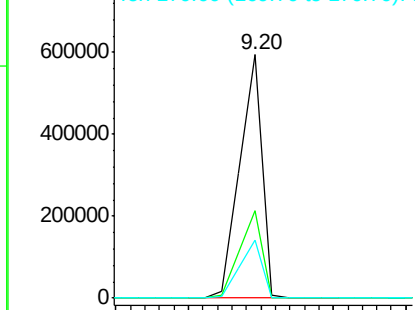


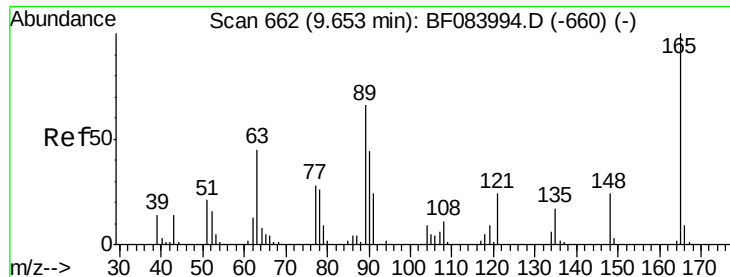

#50
 2,6-Dinitrotoluene
 Concen: 7.57 ng
 RT: 9.87 min Scan# 681
 Delta R.T. 0.22 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53




Instrument :
 BNA_F
 ClientSampleId :
 20151214MGP209BRV46.5


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	28.8	43.2#
89	0.0	35.1	52.7#

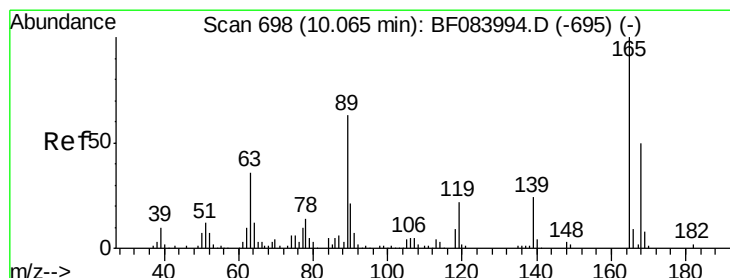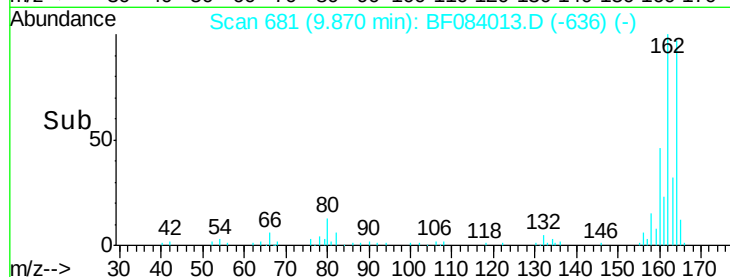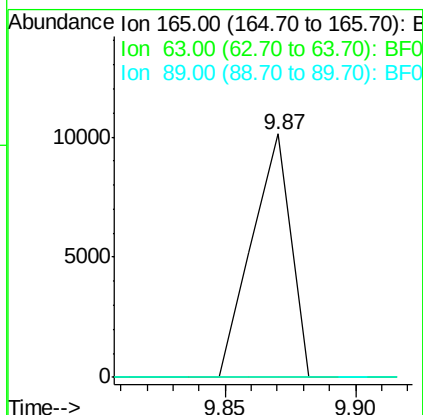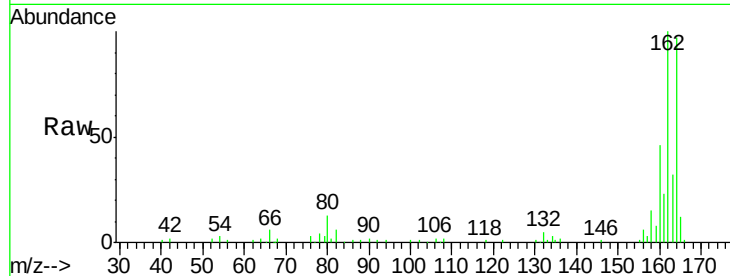

#56
 2,4-Dinitrotoluene
 Concen: 6.02 ng
 RT: 9.87 min Scan# 681
 Delta R.T. -0.19 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.7	55.1#
89	0.0	61.9	92.9#
182	0.0	2.0	3.0#

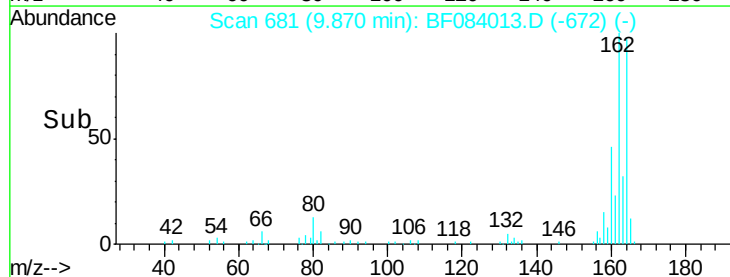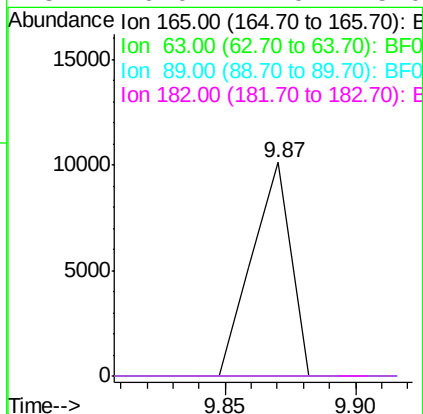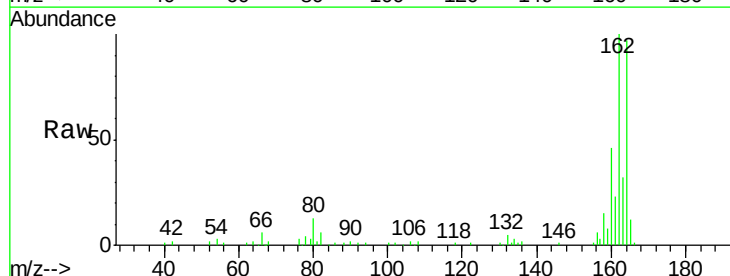


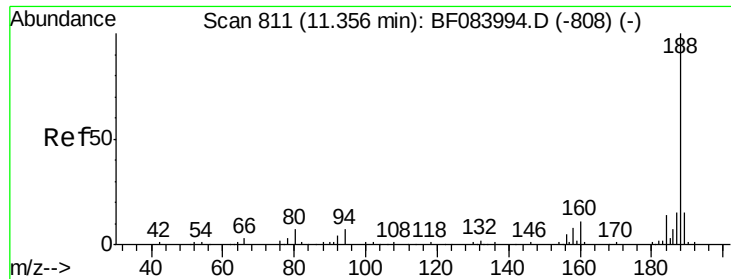




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.36 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Instrument :
 BNA_F
 ClientSampleId :
 20151214MGP209BRV46.5

Tgt Ion:188 Resp: 163002
 Ion Ratio Lower Upper
 188 100
 94 6.0 9.0 13.4#
 80 5.8 9.6 14.4#




Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

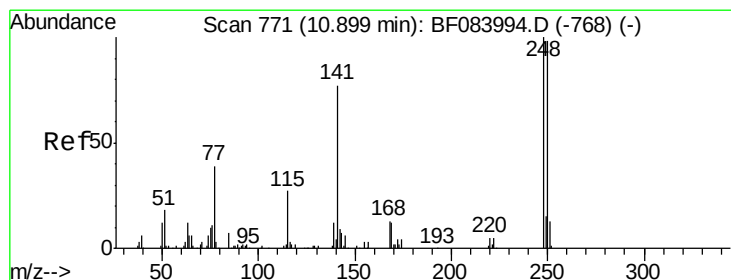
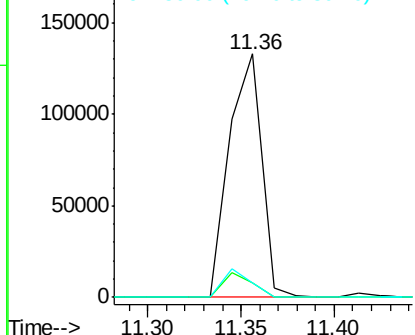



#66
 4-Bromophenyl-phenylether
 Concen: 5.45 ng
 RT: 10.66 min Scan# 750
 Delta R.T. -0.24 min
 Lab File: BF084013.D
 Acq: 23 Dec 2015 2:53

Tgt Ion:248 Resp: 10181
 Ion Ratio Lower Upper
 248 100
 250 185.8 78.4 117.6#
 141 484.6 44.0 66.0#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

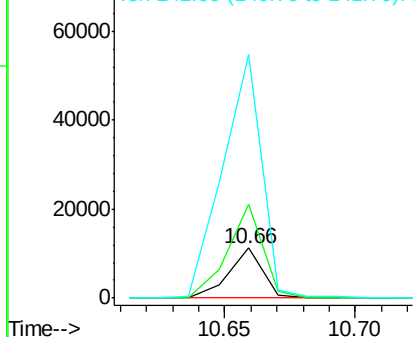

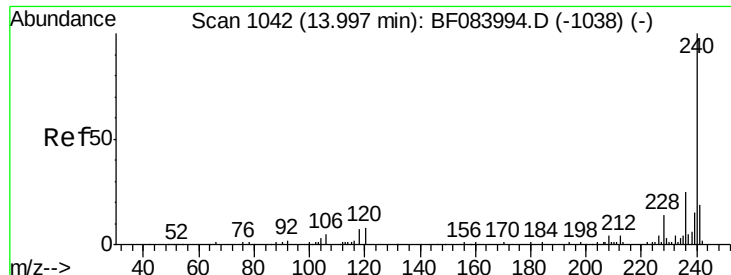

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.99 min Scan# 1041

Delta R.T. -0.01 min

Lab File: BF084013.D

Acq: 23 Dec 2015 2:53





Instrument :

BNA_F

ClientSampleId :

20151214MGP209BRV46.5

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.6	9.5	14.3#
236	24.9	20.6	31.0

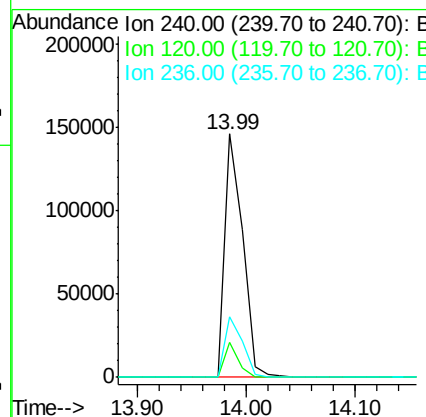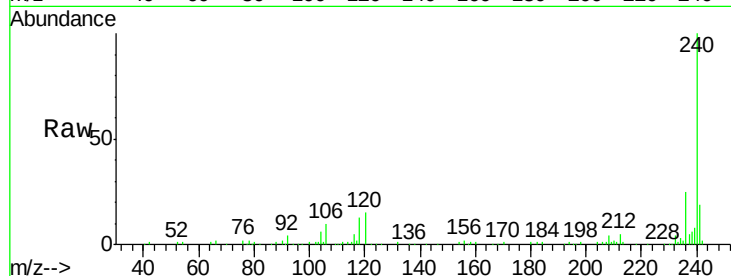

#78

Terphenyl-d14

Concen: 93.14 ng




RT: 12.93 min Scan# 949


Delta R.T. -0.00 min

Lab File: BF084013.D

Acq: 23 Dec 2015 2:53

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.8	5.7	8.5
122	15.1	7.4	11.0#

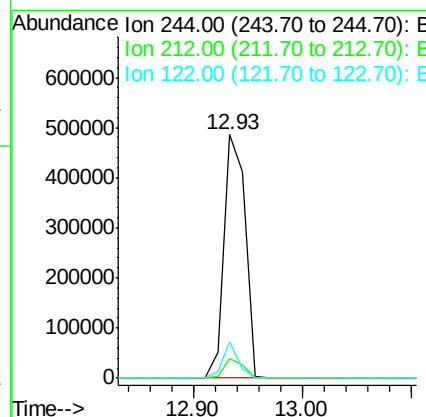

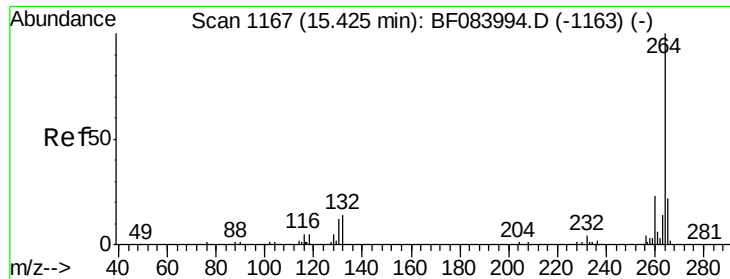

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.41 min Scan# 1166
Delta R.T. -0.01 min
Lab File: BF084013.D
Acq: 23 Dec 2015 2:53

Instrument :
BNA_F
ClientSampleId :
20151214MGP209BRV46.5

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.4	29.2
265	21.7	17.8	26.6

