



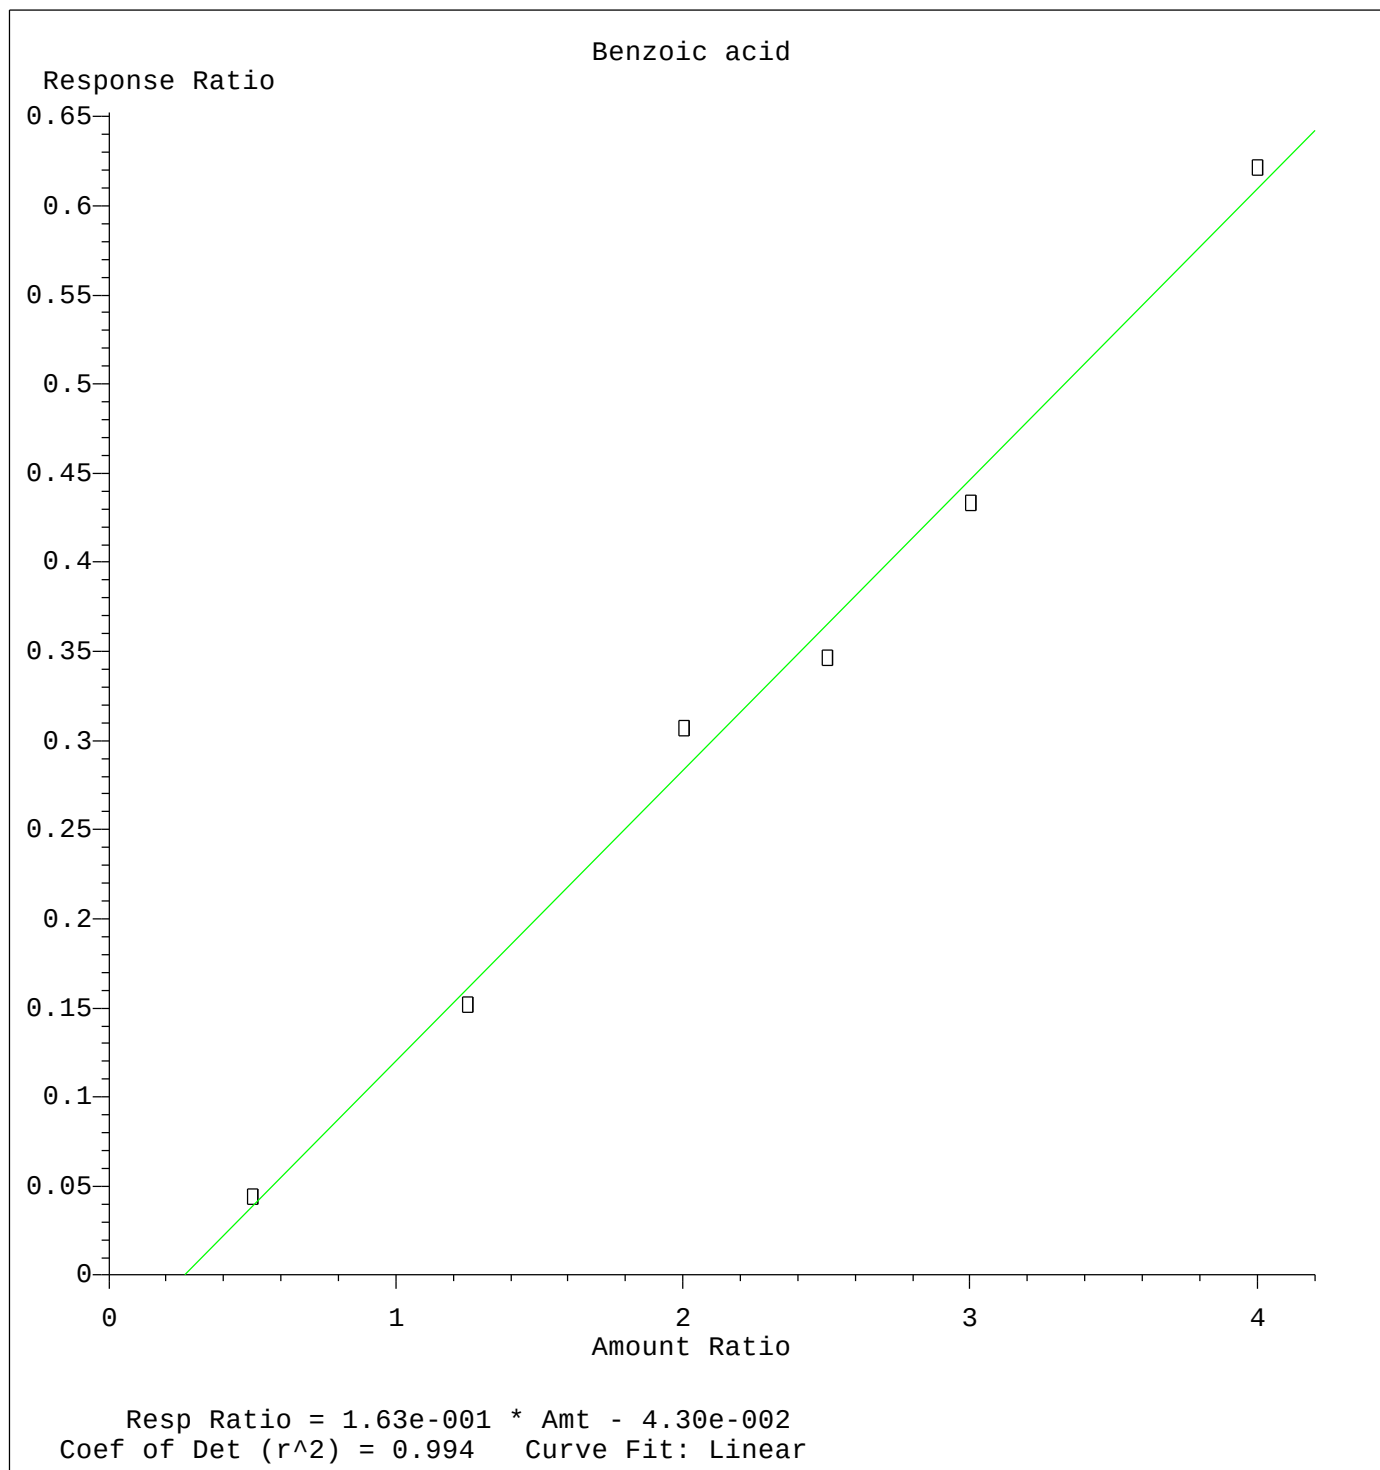

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
Calibration Table Last Updated: Tue Dec 22 18:54:09 2015


Hexachlorocyclopentadiene

Response Ratio

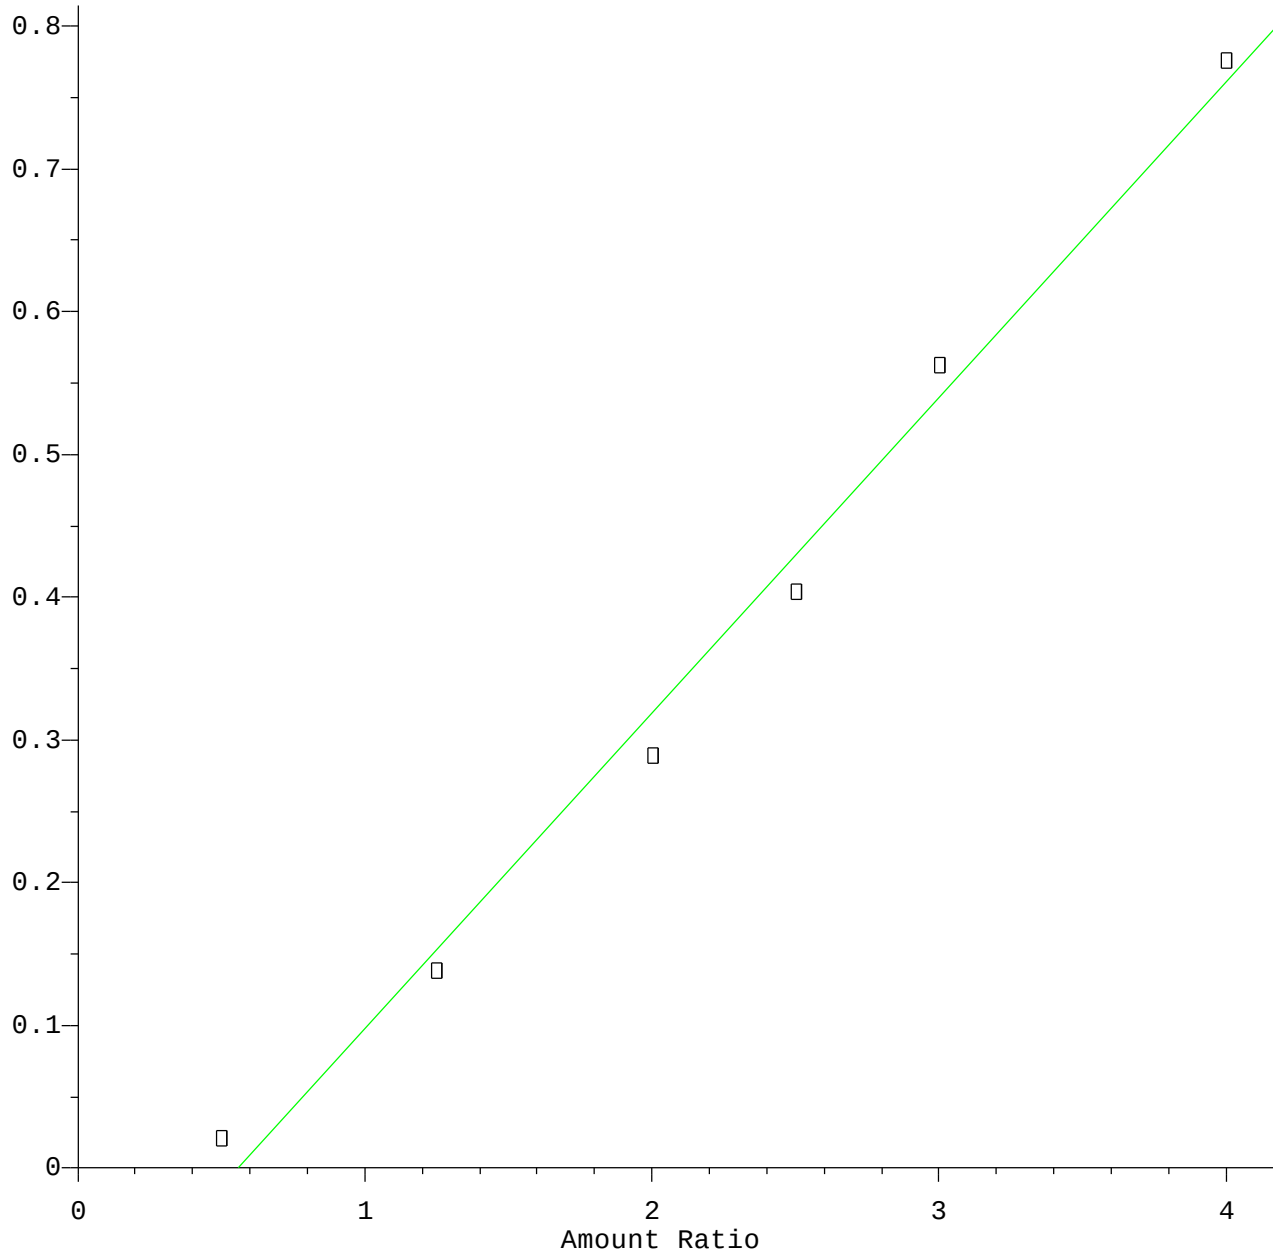


Resp Ratio = $2.21 \times 10^{-1} \times \text{Amt} - 1.23 \times 10^{-1}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
Calibration Table Last Updated: Tue Dec 22 18:54:09 2015

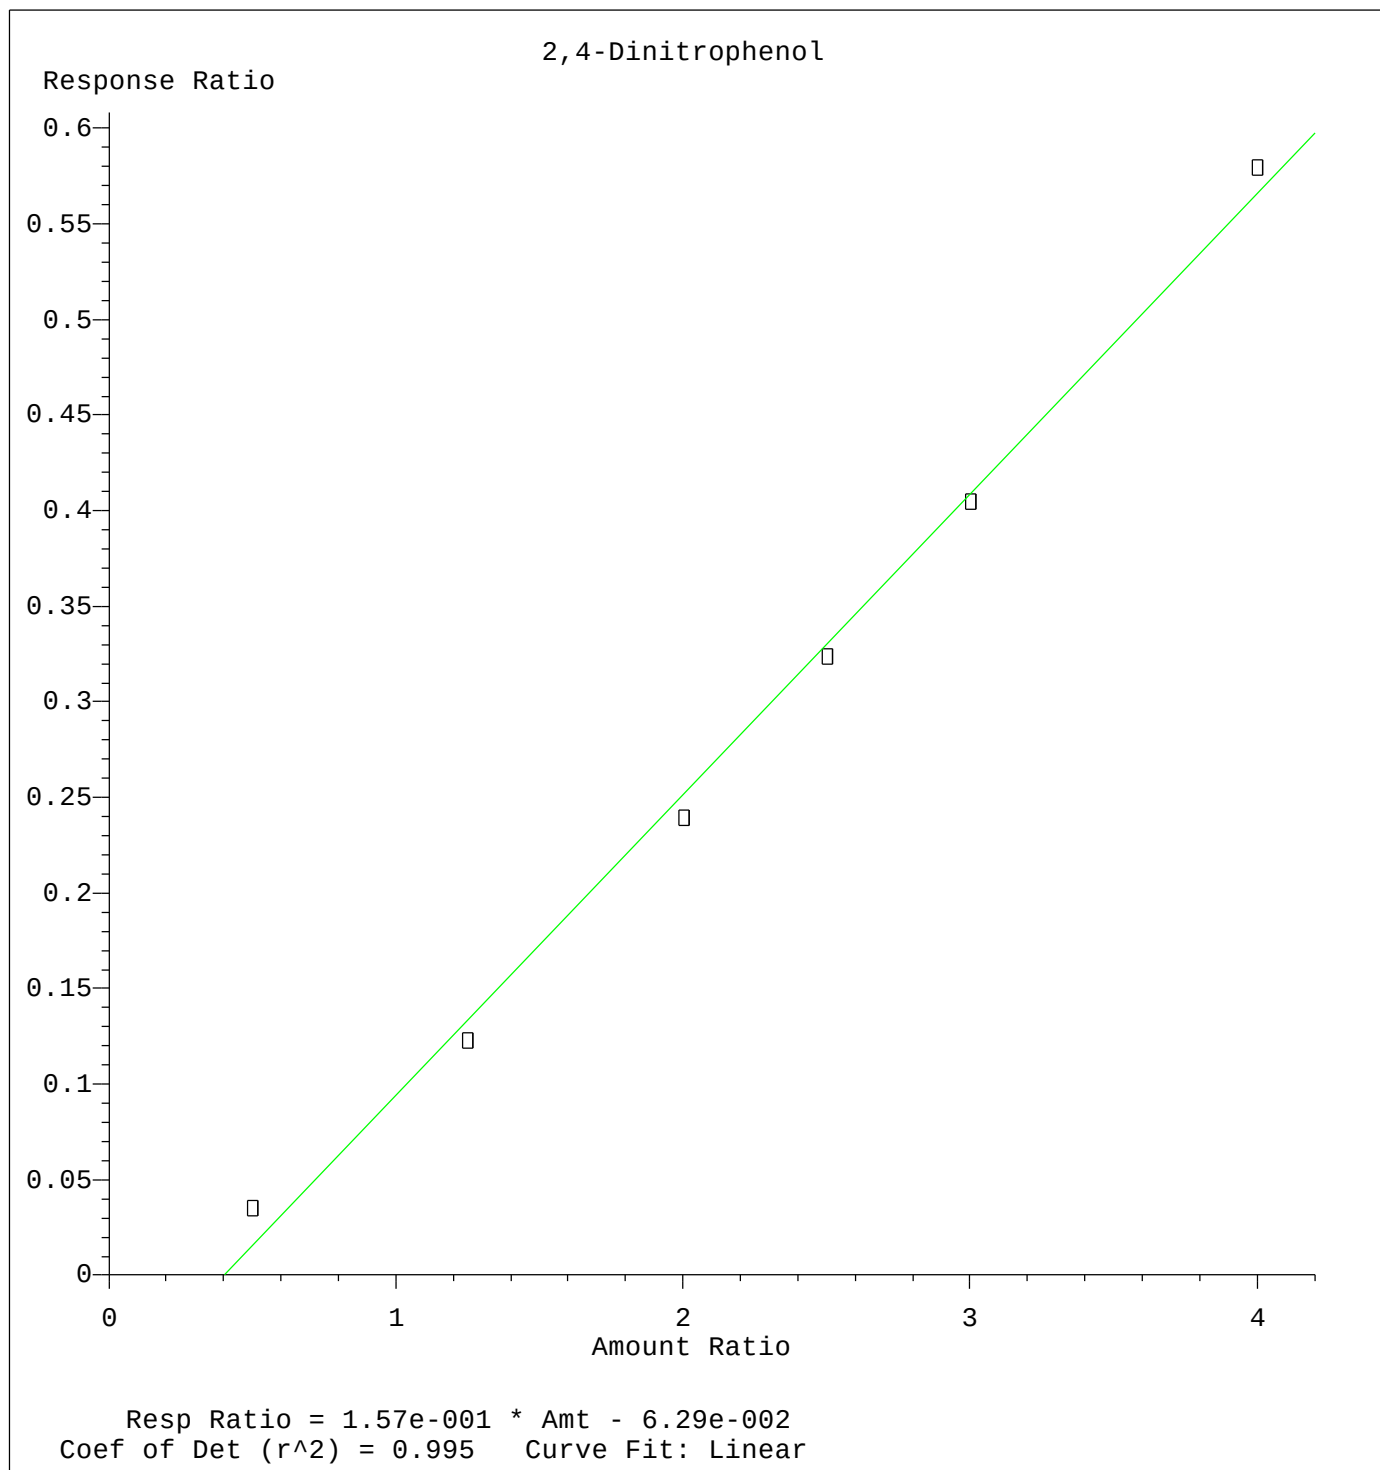

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
Calibration Table Last Updated: Tue Dec 22 18:54:09 2015

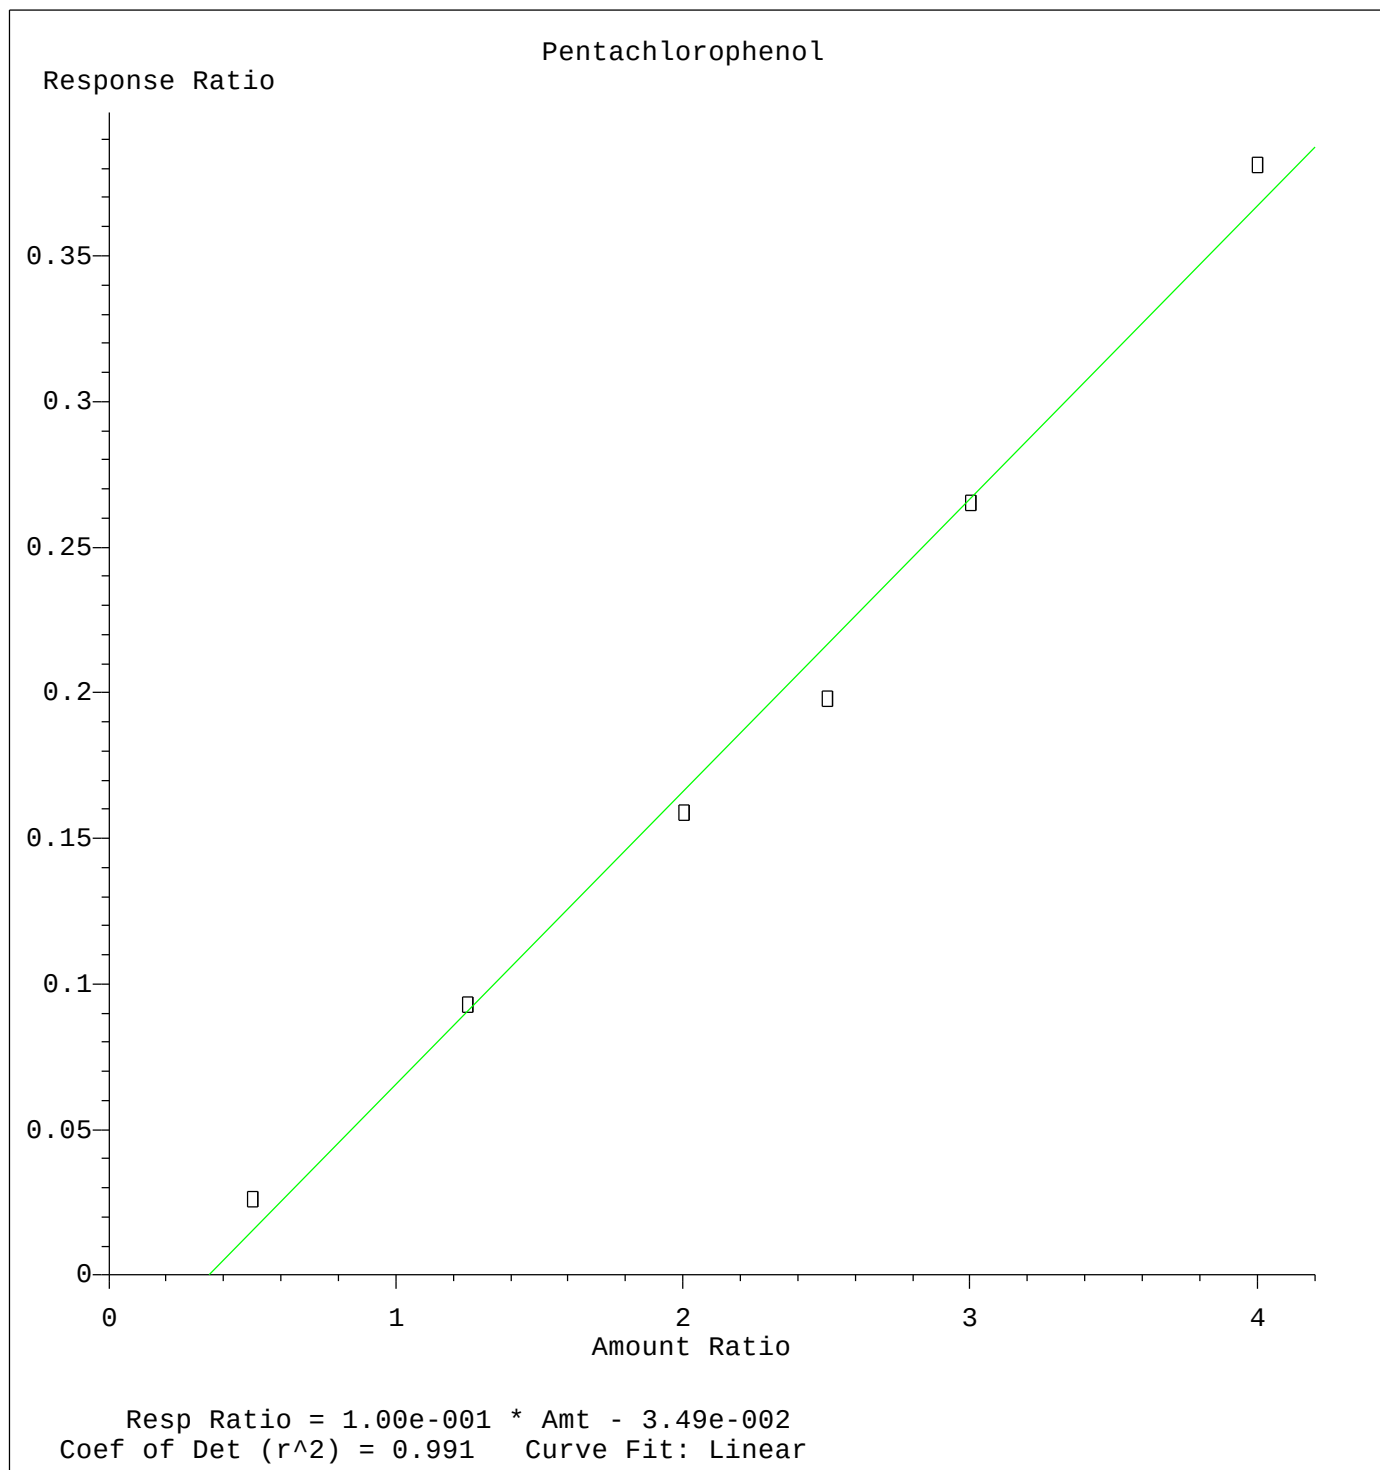

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
Calibration Table Last Updated: Tue Dec 22 18:54:09 2015