
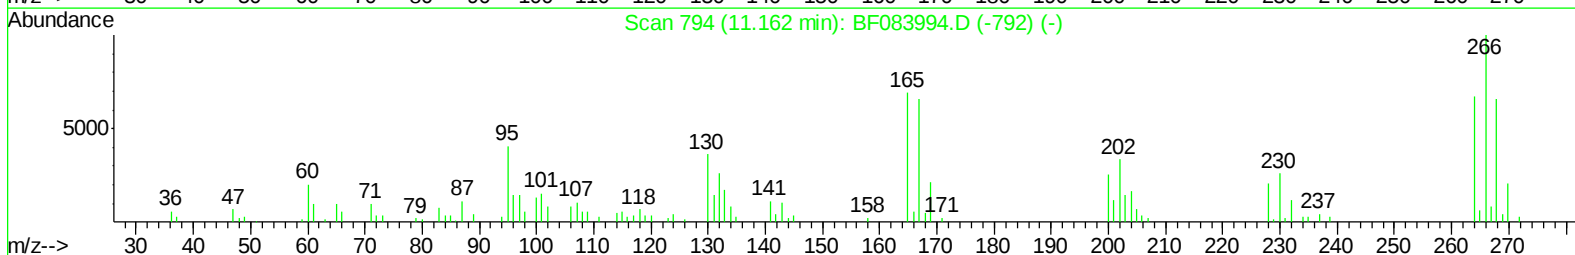
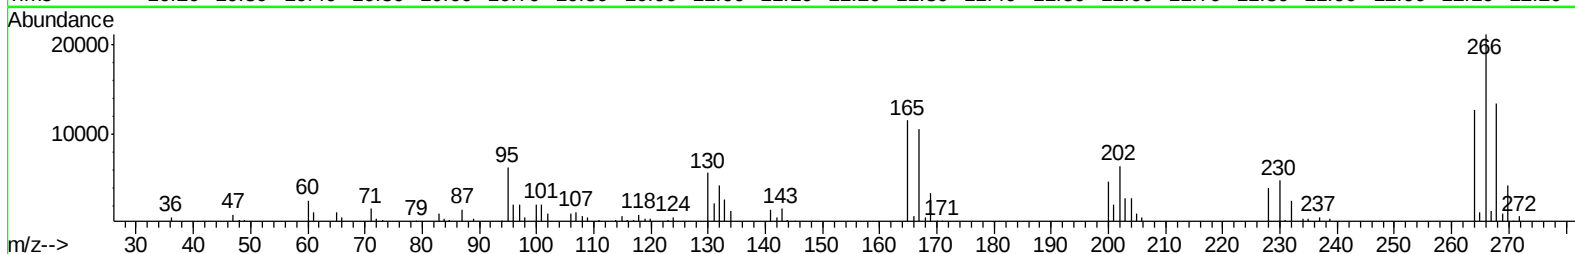


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122215\
Data File : BF084025.D
Acq On : 23 Dec 2015 8:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 18:21:18 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 18:54:09 2015
Response via : Initial Calibration

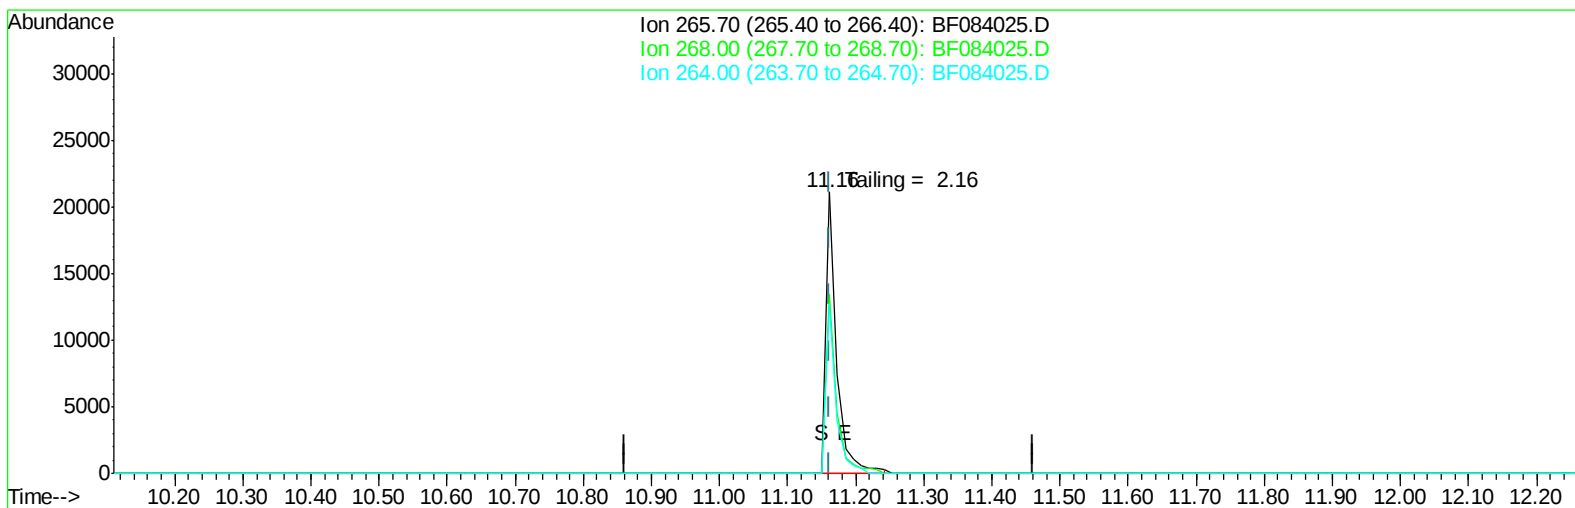

TIC: BF084025.D

(69) Pentachlorophenol (C)




11.162min (-0.000) 0.00ng

response 22674

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	63.82
264.00	62.70	60.21
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122215\
 Data File : BF084025.D
 Acq On : 23 Dec 2015 8:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 18:21:18 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 22 18:54:09 2015
 Response via : Initial Calibration

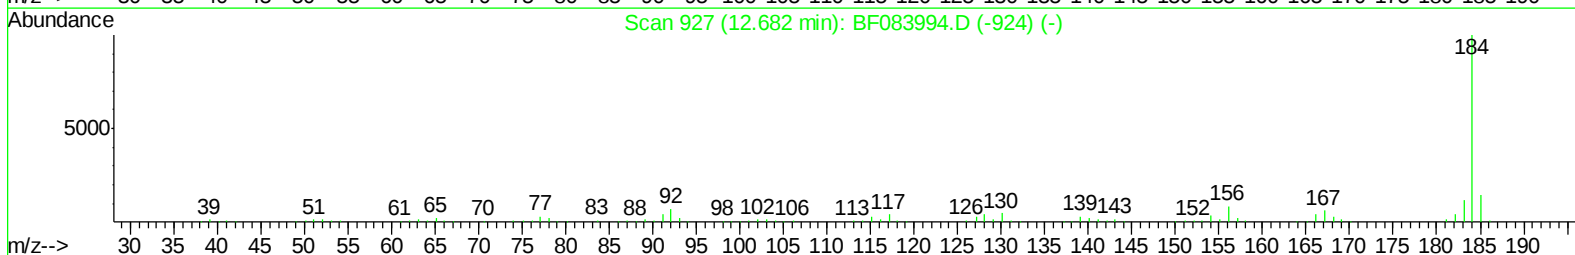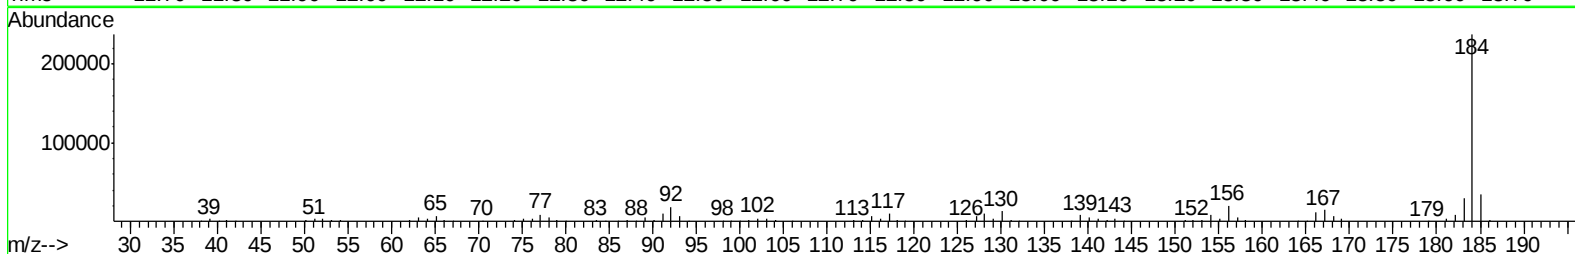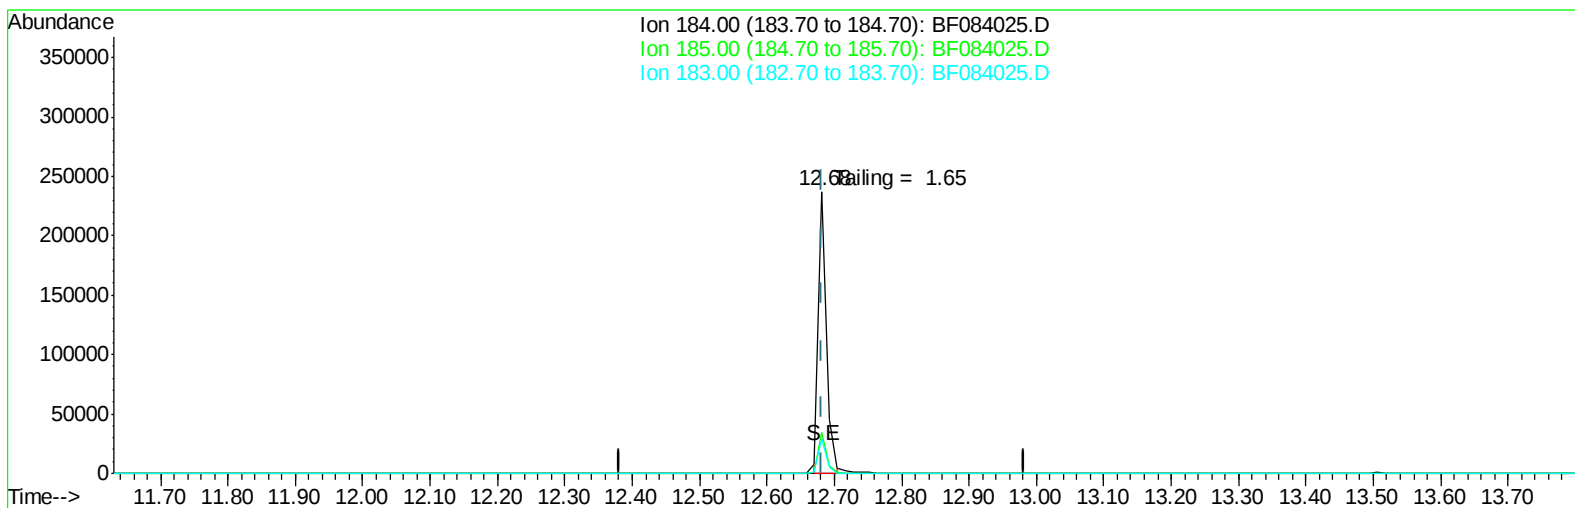

TIC: BF084025.D

(76) Benzidine

12.682min (-0.000) 0.00ng

response 205964

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.51
183.00	12.30	12.27
0.00	0.00	0.00