
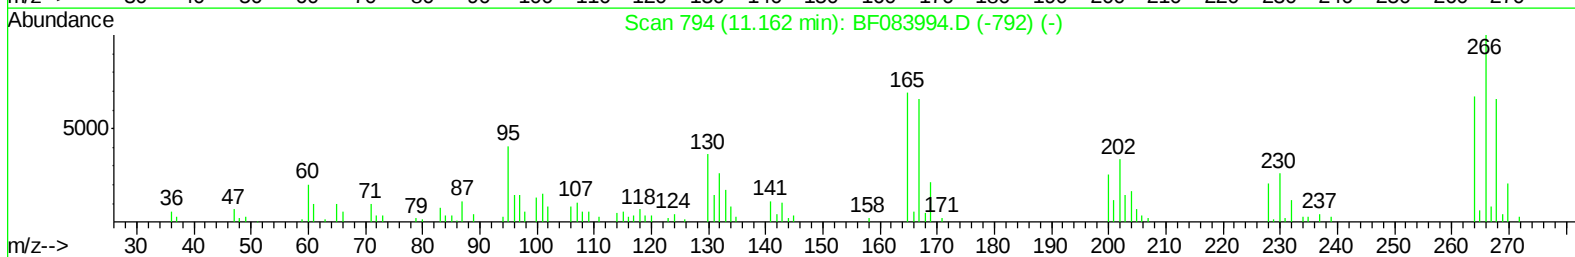
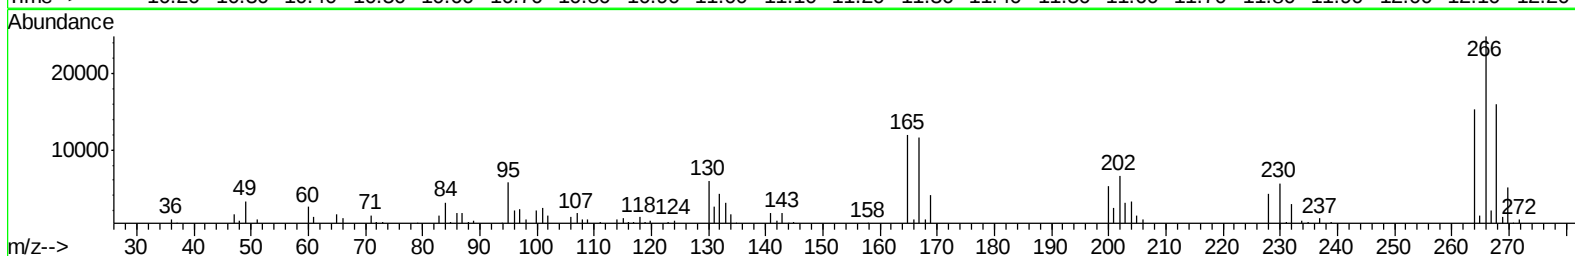


Data Path : Z:\HPCHEM1\BNA F\Data\BF122215\
Data File : BF083990.D
Acq On : 22 Dec 2015 14:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:33:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 18:54:09 2015
Response via : Initial Calibration

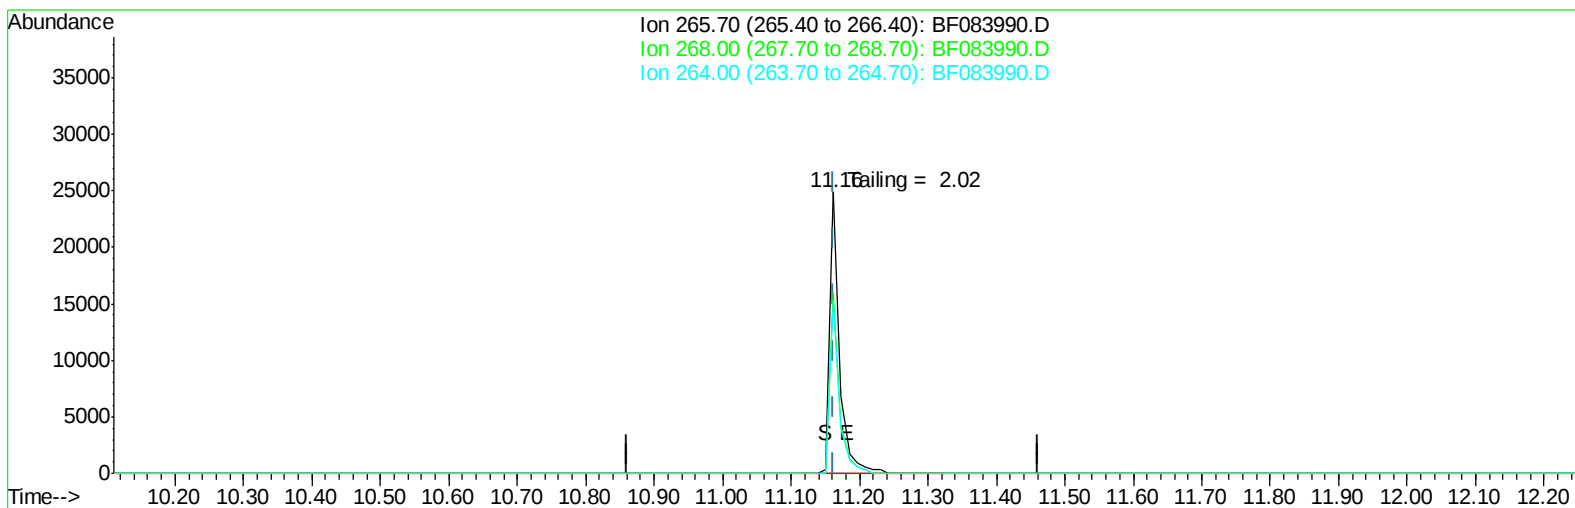

TIC: BF083990.D

(69) Pentachlorophenol (C)

11.162min (+0.000) 0.00ng

response 24562

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	64.31
264.00	62.70	61.59
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\Data\BF122215\  
Data File : BF083990.D  
Acq On    : 22 Dec 2015  14:25  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Data File : BF083990.D

Acq On : 22 Dec 2015 14:25

Operator : UM/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1


Quant Time: Dec 23 05:33:04 2015

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122215.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

0Last Update : Tue Dec 22 18:54:09 2015

Response via : Initial Calibration

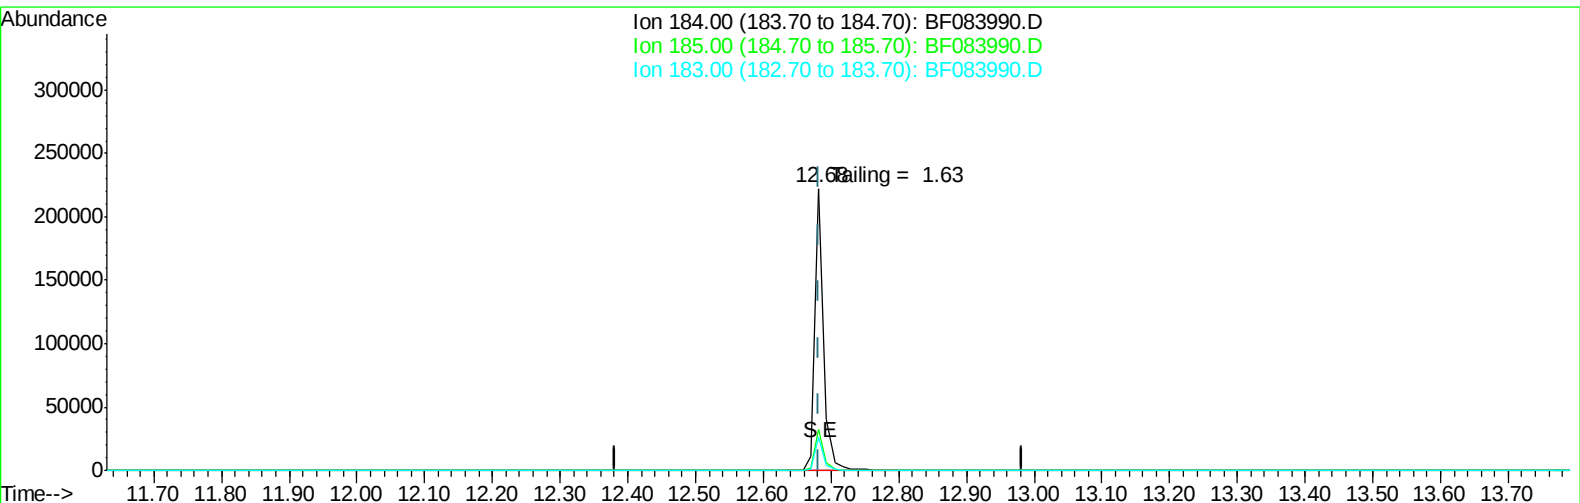

lon 184.00 (183.70 to 184.70): BF083990.D

Ion 185.00 (184.70 to 185.70): BF083990.D

Ion 183.00 (182.70 to 183.70): BF083990.D


12.618 $\tau_{\text{ailing}} = 1.63$

12.618 $\tau_{\text{ailing}} = 1.63$


5

5

Time--> 11.70 11.80 11.90 12.00 12.10 12.20 12.30 12.40 12.50 12.60 12.70 12.80 12.90 13.00 13.10 13.20 13.30 13.40 13.50 13.60 13.70

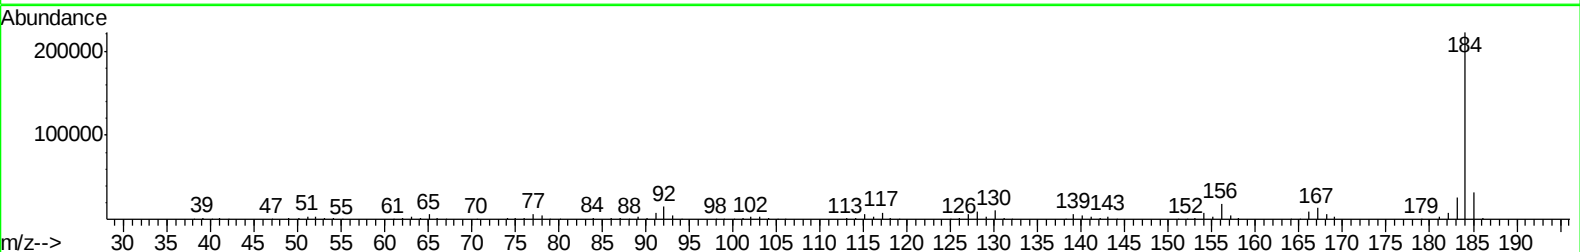

m/z--> 30 35 40 45 50 55 60 65 70 75 80 85 90 95 100 105 110 115 120 125 130 135 140 145 150 155 160 165 170 175 180 185 190

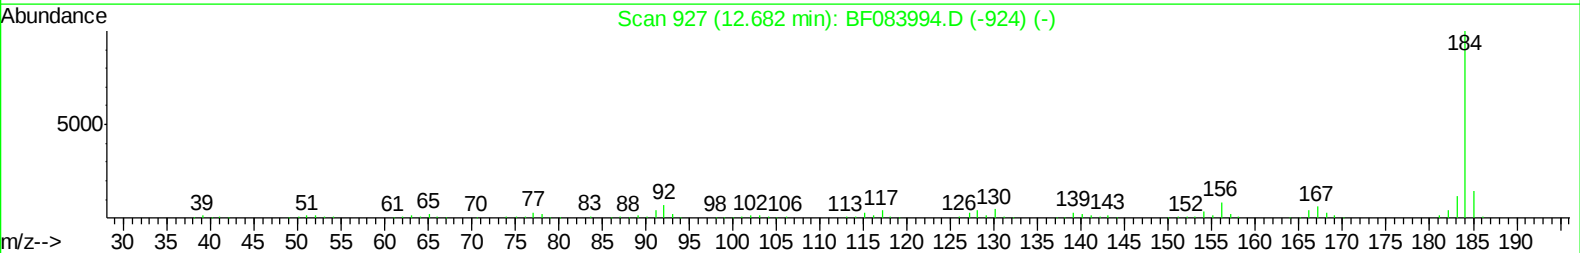

Scan 927 (12.682 min): BF083994.D (-924) (-)

m/z--> 30 35 40 45 50 55 60 65 70 75 80 85 90 95 100 105 110 115 120 125 130 135 140 145 150 155 160 165 170 175 180 185 190

TIC: BF083990.D

(76) Benzidine

12.682min (-0.000) 0.00ng

response 197230

Ion	Exp%	Act%
-----	------	------

184.00	100	100
--------	-----	-----

185.00	15.20	14.74
--------	-------	-------

183.00	12.30	11.85
--------	-------	-------

0.00 0.00 0.00