
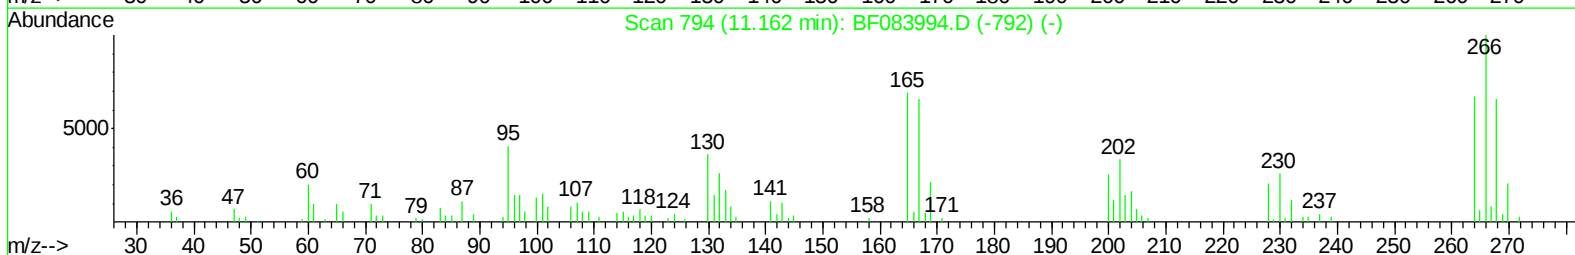
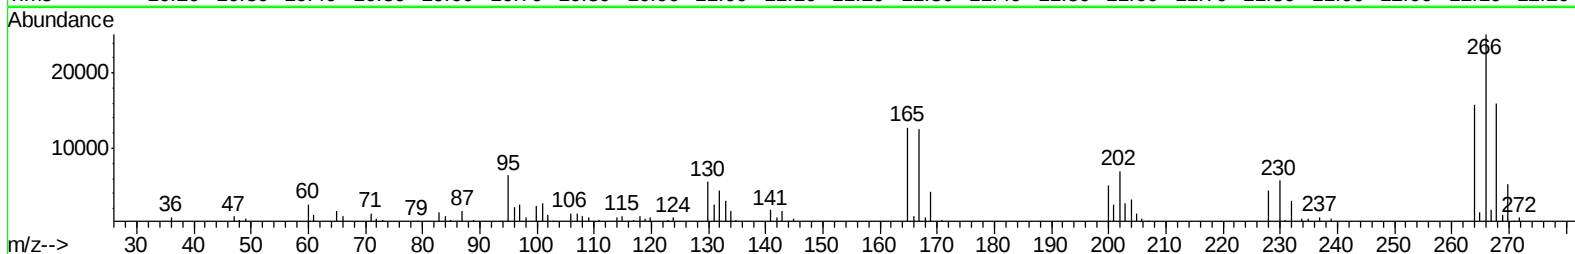


Data Path : Z:\HPCHEM1\BNA F\Data\BF122215\
Data File : BF083999.D
Acq On : 22 Dec 2015 19:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:34:16 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 18:54:09 2015
Response via : Initial Calibration

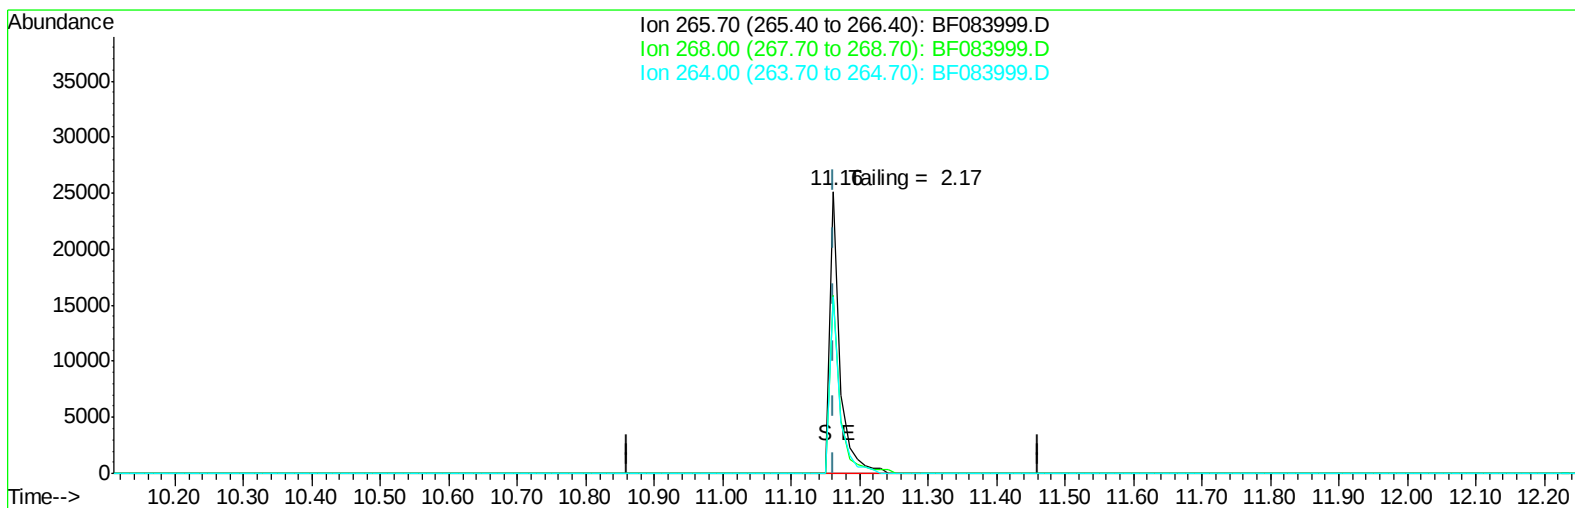

TIC: BF083999.D

(69) Pentachlorophenol (C)




11.162min (-0.000) 0.00ng

response 25532

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	63.33
264.00	62.70	62.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF122215\
Data File : BF083999.D
Acq On : 22 Dec 2015 19:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:34:16 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 18:54:09 2015
Response via : Initial Calibration

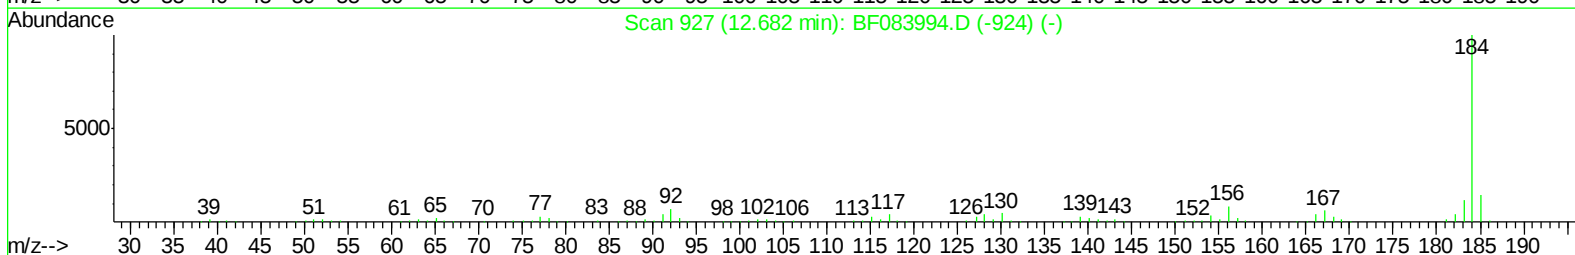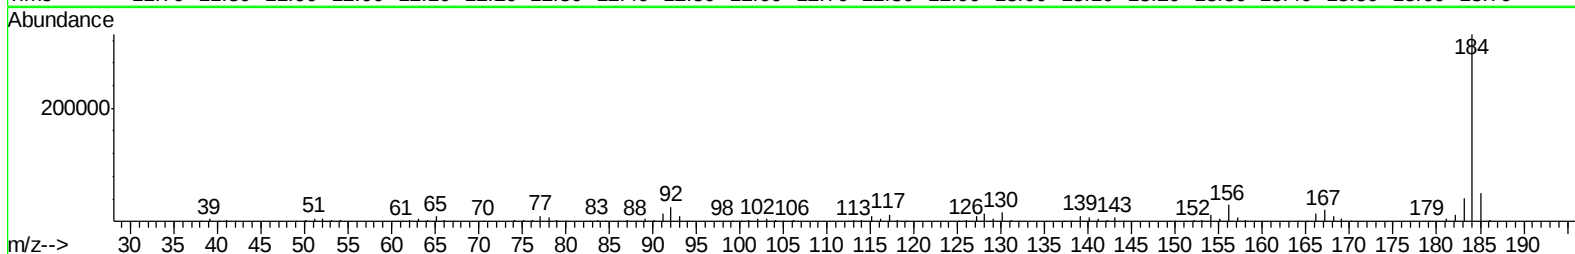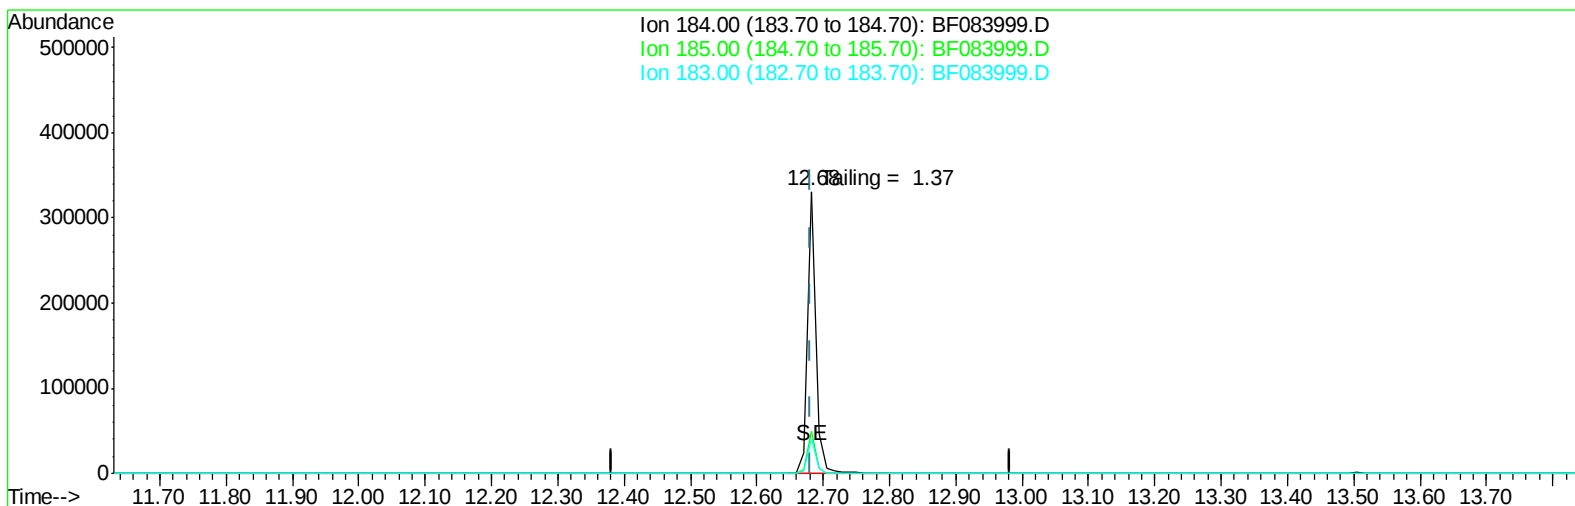

TIC: BF083999.D

(76) Benzidine

12.682min (-0.000) 0.00ng

response 284869

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.01
183.00	12.30	12.12
0.00	0.00	0.00