


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122215\
 Data File : BF083990.D
 Acq On : 22 Dec 2015 14:25
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 22 18:54:09 2015

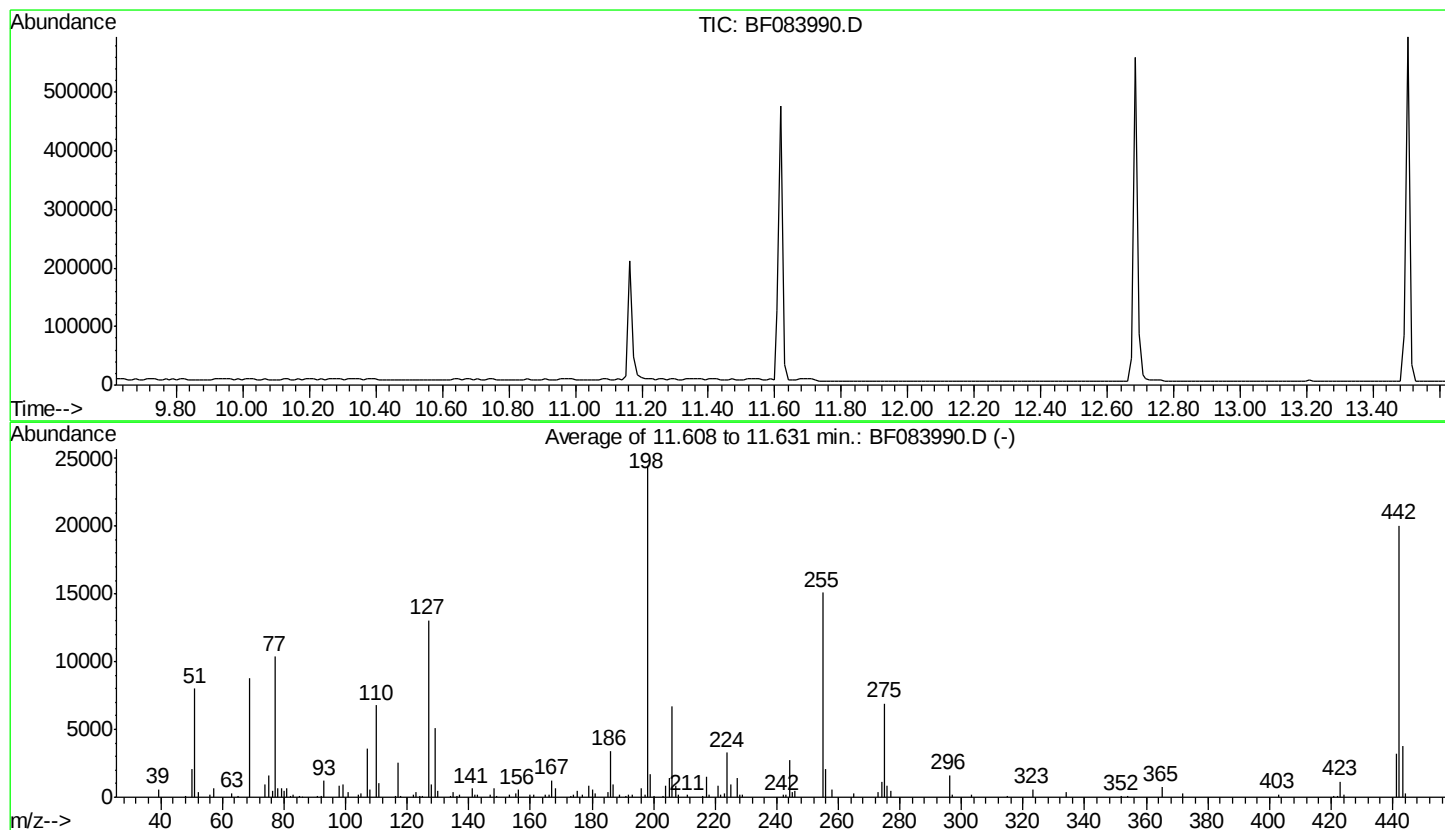

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	8022	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.8	8754	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	13033	PASS
197	198	0.00	2	0.9	216	PASS
198	198	100	100	100.0	24463	PASS
199	198	5	9	6.8	1667	PASS
275	198	10	60	28.3	6917	PASS
365	198	1	100	3.2	785	PASS
441	442	0.01	24	15.9	3176	PASS
442	198	50	100	81.8	20022	PASS
443	442	15	24	18.7	3739	PASS