
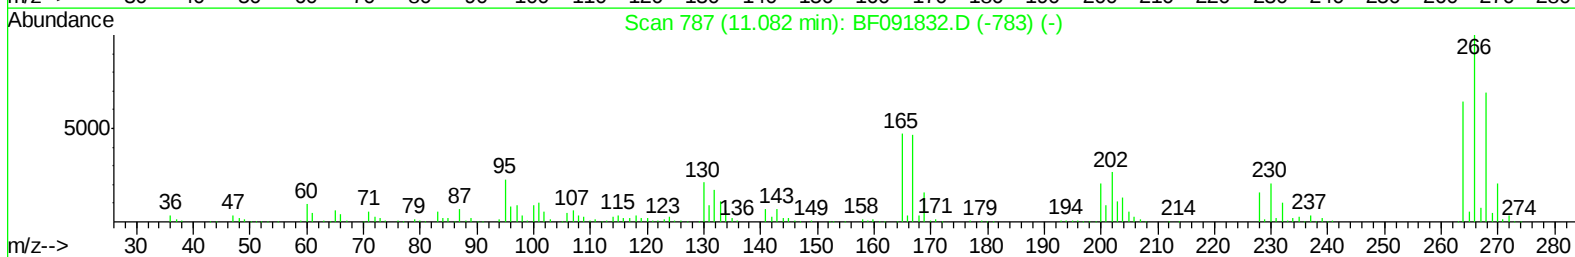
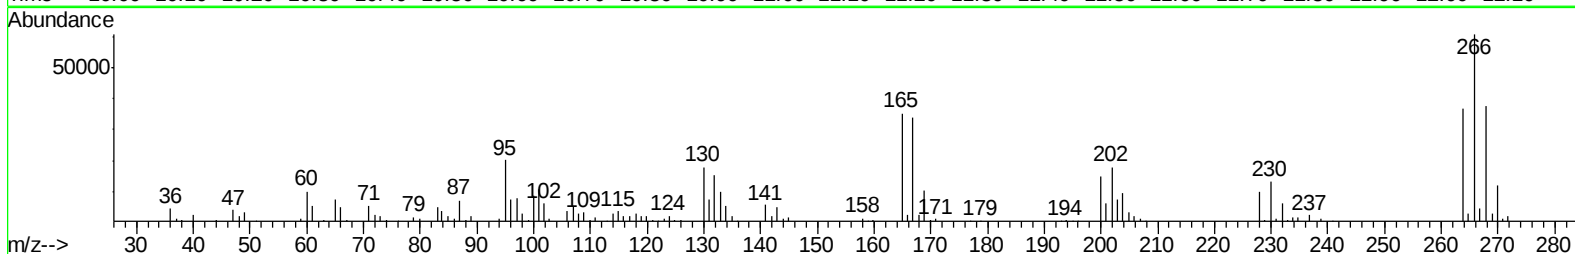


Data Path : Z:\HPCHEM1\BNA_F\Data\BF122216\
Data File : BF091876.D
Acq On : 22 Dec 2016 10:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 07:26:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 17:32:10 2016
Response via : Initial Calibration

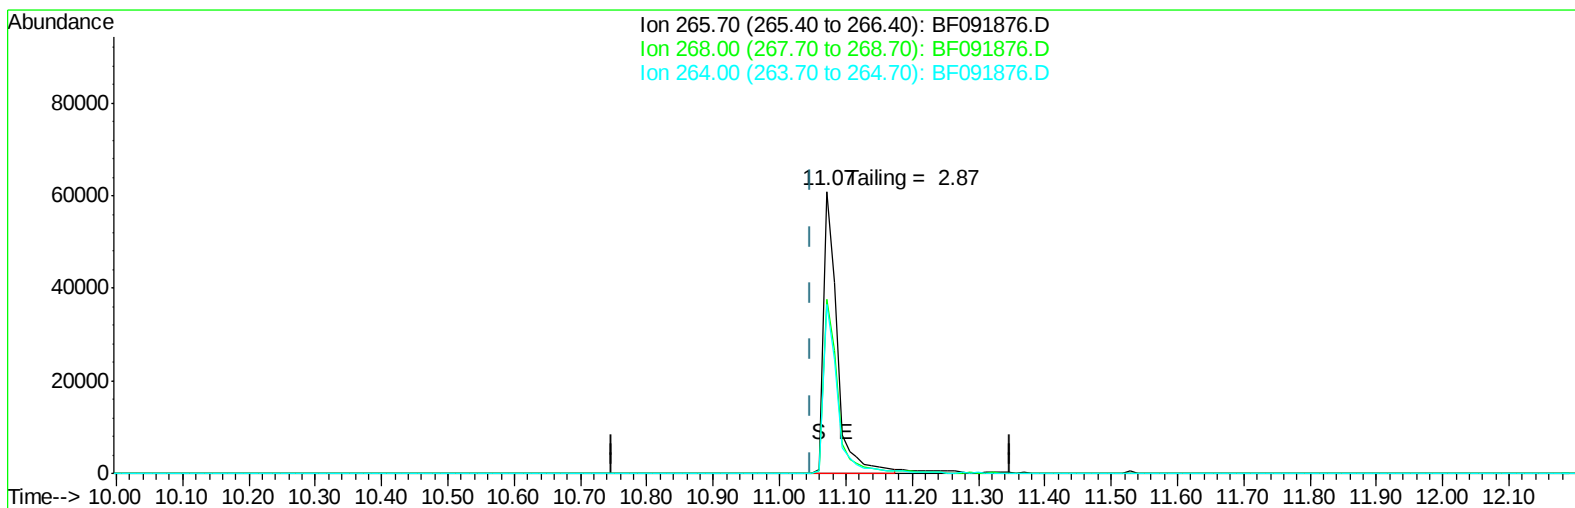

TIC: BF091876.D

(69) Pentachlorophenol (C)




11.071min (+0.023) 36172.64ng

response 88018

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.05
264.00	62.90	60.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF122216\
 Data File : BF091876.D
 Acq On : 22 Dec 2016 10:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 07:26:56 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 17:32:10 2016
 Response via : Initial Calibration

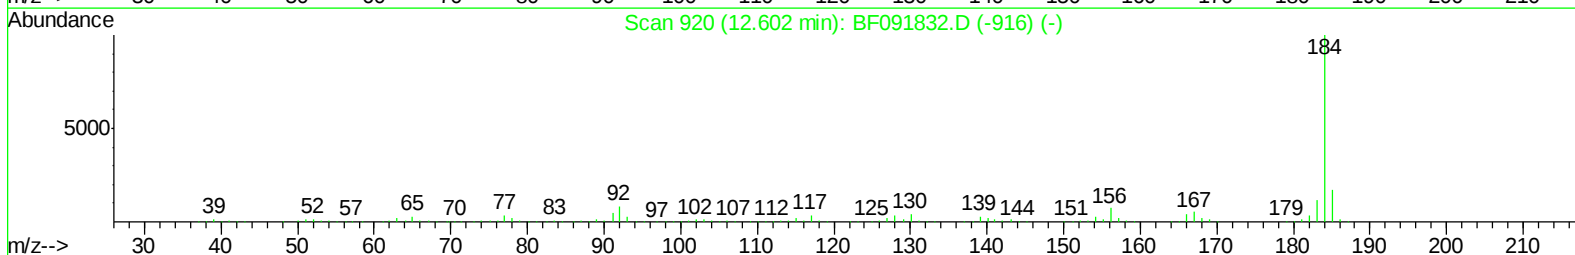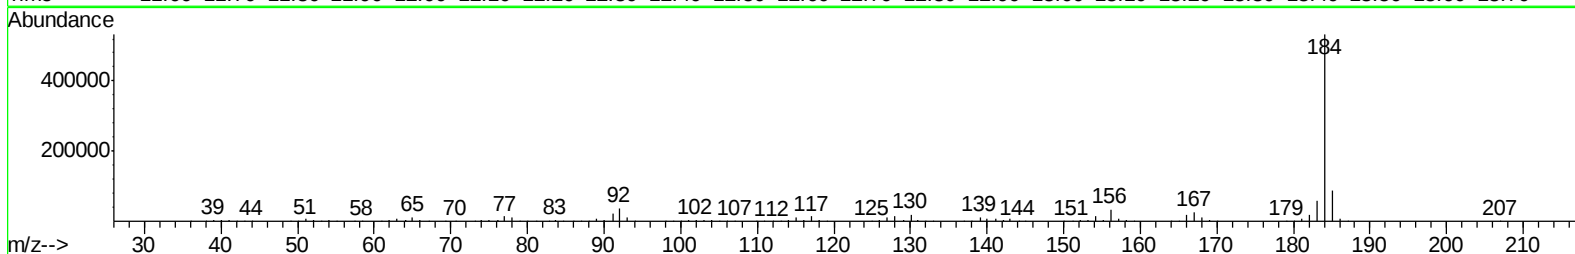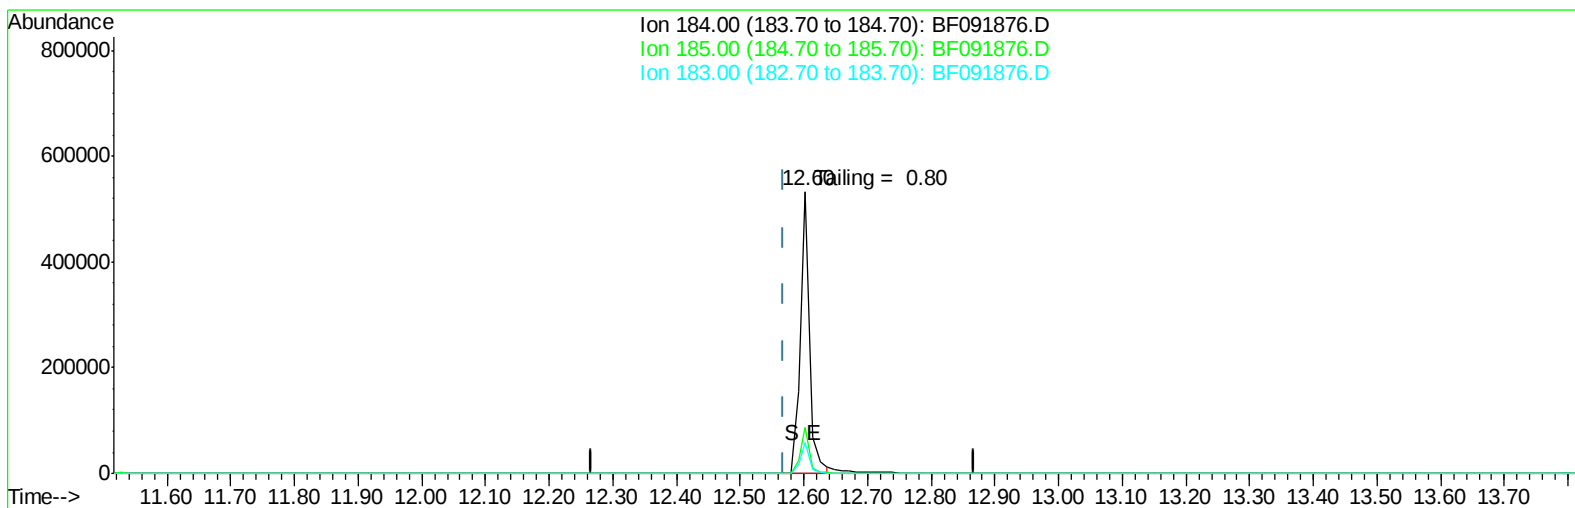

TIC: BF091876.D

(76) Benzidine

12.602min (+0.034) -20.00ng

response 569103

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.40
183.00	11.50	10.77
0.00	0.00	0.00