

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122216\
 Data File : BF091904.D
 Acq On : 23 Dec 2016 4:39
 Operator : UM/SJ
 Sample : H6182-06RE
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-52(0-1)-121916RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.613	37	46	49	rBV	362627	858580	3.38%	0.272%
2	2.693	49	53	55	rVV	109589	258803	1.02%	0.082%
3	2.738	55	57	60	rVB	169022	282541	1.11%	0.090%
4	2.955	67	76	82	rVB3	133086	521818	2.05%	0.166%
5	3.138	88	92	103	rVB2	192647	506144	1.99%	0.161%
6	3.401	109	115	123	rVB	318639	994312	3.91%	0.315%
7	3.641	132	136	139	rVV	182615	400177	1.57%	0.127%
8	3.744	139	145	148	rVV	470242	1068126	4.20%	0.339%
9	3.904	152	159	162	rBV	1933803	4249093	16.72%	1.348%
10	3.961	162	164	169	rVB	893359	1447789	5.70%	0.459%
11	4.076	169	174	176	rBV2	543254	1264478	4.97%	0.401%
12	4.133	176	179	183	rVB	779004	1527706	6.01%	0.485%
13	4.281	188	192	198	rBV2	1771387	3447834	13.56%	1.094%
14	4.396	198	202	206	rVB	1111907	1688977	6.64%	0.536%
15	4.499	209	211	214	rVB	356025	582888	2.29%	0.185%
16	4.579	214	218	220	rBV2	443090	823070	3.24%	0.261%
17	4.624	220	222	224	rBV	772280	1084674	4.27%	0.344%
18	4.659	224	225	227	rVB2	227584	268068	1.05%	0.085%
19	4.750	227	233	235	rBV	2924014	5271653	20.74%	1.672%
20	4.784	235	236	237	rBV	268425	359153	1.41%	0.114%
21	4.841	238	241	244	rBV2	4983746	8701592	34.23%	2.760%
22	4.910	244	247	249	rBV	5165674	6667421	26.23%	2.115%
23	5.047	257	259	263	rVB2	905690	1457861	5.74%	0.462%
24	5.127	263	266	267	rBV	4487774	7557040	29.73%	2.397%
25	5.150	267	268	275	rVB3	1915213	5148313	20.25%	1.633%
26	5.253	275	277	279	rBV	225867	294013	1.16%	0.093%
27	5.299	279	281	283	rBV	1201713	1862411	7.33%	0.591%
28	5.333	283	284	285	rVB	497102	340763	1.34%	0.108%
29	5.401	287	290	294	rBV2	3494603	7338896	28.87%	2.328%
30	5.504	296	299	301	rBV	3762195	7426984	29.22%	2.356%
31	5.550	301	303	305	rBV	3689607	4264673	16.78%	1.353%
32	5.596	305	307	311	rVB2	3640076	7257243	28.55%	2.302%
33	5.664	311	313	318	rVB	1852161	3487226	13.72%	1.106%
34	5.767	318	322	324	rBV2	5010106	12162153	47.85%	3.858%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
 Data File : BF091904.D
 Acq On : 23 Dec 2016 4:39
 Operator : UM/SJ
 Sample : H6182-06RE
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-52(0-1)-121916RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	5.813	324	326	331	rBV4	1443346	3841788	15.11%	1.219%
36	5.904	331	334	337	rBV2	5581302	12462379	49.03%	3.954%
37	5.973	337	340	341	rBV2	1528115	2871458	11.30%	0.911%
38	6.019	341	344	347	rBV3	7445723	20857255	82.06%	6.617%
39	6.076	347	349	358	rVB3	6251957	25418043	100.00%	8.064%
40	6.213	358	361	366	rBV2	3795832	10986711	43.22%	3.485%
41	6.304	366	369	374	rBV3	4620023	14686005	57.78%	4.659%
42	6.453	377	382	385	rBV4	2935646	11321999	44.54%	3.592%
43	6.556	385	391	395	rBV5	4658692	24112672	94.86%	7.649%
44	10.488	732	735	737	rVB	4812781	8923381	35.11%	2.831%
45	10.739	754	757	760	rVB2	7203994	12365203	48.65%	3.923%
46	10.933	772	774	776	rVB2	1997571	2481253	9.76%	0.787%
47	11.036	781	783	789	rVB5	1378185	3173400	12.48%	1.007%
48	11.185	793	796	798	rVB	3067240	5045637	19.85%	1.601%
49	11.276	802	804	812	rVB3	1190611	3097656	12.19%	0.983%
50	11.528	822	826	828	rBV5	1137686	2792679	10.99%	0.886%
51	11.573	828	830	831	rVB	896256	1032314	4.06%	0.327%
52	11.608	831	833	836	rVB4	482543	765940	3.01%	0.243%
53	11.665	836	838	840	rVB	1946792	2389822	9.40%	0.758%
54	11.768	844	847	849	rBV2	1181963	1598392	6.29%	0.507%
55	11.859	853	855	861	rVV5	2477274	5547106	21.82%	1.760%
56	11.962	861	864	867	rVV3	1294683	2885030	11.35%	0.915%
57	12.031	867	870	871	rVV3	1508716	3611604	14.21%	1.146%
58	12.054	871	872	875	rVV	3205935	4716399	18.56%	1.496%
59	12.111	875	877	882	rVB4	1207600	2828144	11.13%	0.897%
60	12.214	883	886	888	rBV	1297917	2469033	9.71%	0.783%
61	12.305	891	894	899	rVV2	3074564	6396024	25.16%	2.029%
62	12.396	900	902	905	rVB	1201971	1423277	5.60%	0.452%
63	12.522	910	913	917	rVB3	1453865	1922165	7.56%	0.610%
64	12.579	917	918	919	rBV	460427	384581	1.51%	0.122%
65	12.648	922	924	928	rVB4	310670	508892	2.00%	0.161%
66	12.819	937	939	941	rBV	1442227	2599126	10.23%	0.825%
67	12.854	941	942	945	rVB	3155217	3515735	13.83%	1.115%
68	12.991	952	954	957	rVB	1296188	1269493	4.99%	0.403%
69	13.299	979	981	985	rBV3	173931	385025	1.51%	0.122%
70	13.905	1032	1034	1035	rVB	897331	953544	3.75%	0.302%
71	15.300	1153	1156	1160	rBV	609047	1066544	4.20%	0.338%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
Data File : BF091904.D
Acq On : 23 Dec 2016 4:39
Operator : UM/SJ
Sample : H6182-06RE
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-52(0-1)-121916RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	17.197	1317	1322	1327	rVB4	286768	864336	3.40%	0.274%
73	17.586	1353	1356	1361	rVB3	118982	284006	1.12%	0.090%
74	17.803	1373	1375	1386	rVB2	186458	496304	1.95%	0.157%


Sum of corrected areas: 315222828

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122216\
Data File : BF091904.D
Acq On : 23 Dec 2016 4:39
Operator : UM/SJ
Sample : H6182-06RE
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-52(0-1)-121916RE

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

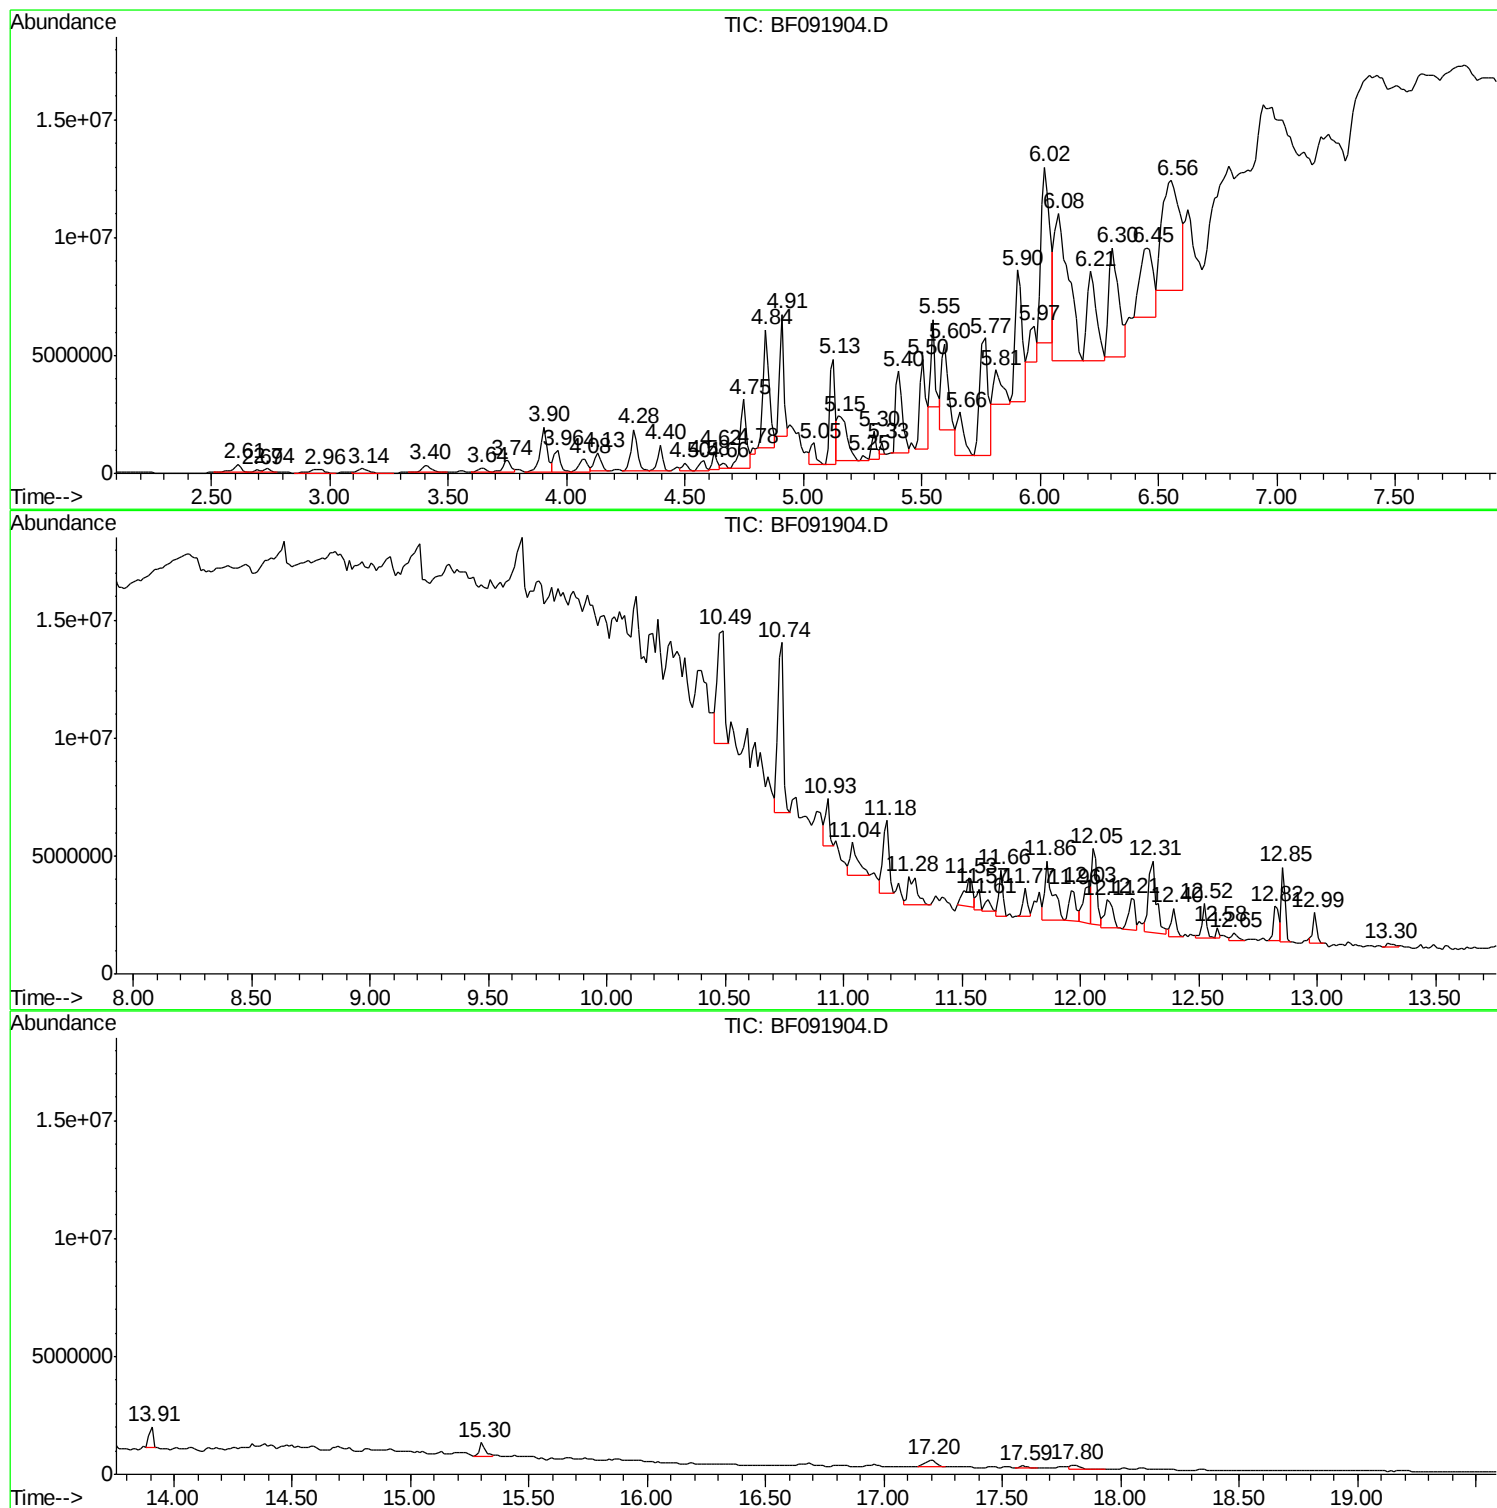

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
Data_File : BF091904.D
Acq_On : 23-Dec-2016 4:399
Operator : UM/SJJ
Sample : H6182-06REE
Misc :
ALS_Vial : 55 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-52(0-1)-121916RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
