

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122216\
 Data File : BF091905.D
 Acq On : 23 Dec 2016 5:06
 Operator : UM/SJ
 Sample : H6182-07RE
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-52(6-8)-121916RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.533	32	39	43	rBV2	169828	492252	5.22%	0.391%
2	2.887	62	70	79	rBV2	220949	691069	7.34%	0.550%
3	3.070	79	86	90	rBV2	239294	627576	6.66%	0.499%
4	3.367	106	112	118	rVB3	60195	223810	2.38%	0.178%
5	3.493	118	123	129	rBV2	237290	657503	6.98%	0.523%
6	3.607	129	133	136	rBV2	84423	214358	2.28%	0.170%
7	3.687	136	140	142	rBV2	74191	178240	1.89%	0.142%
8	3.744	142	145	149	rVB2	132628	318647	3.38%	0.253%
9	3.858	149	155	158	rBV2	449572	1029710	10.93%	0.819%
10	3.916	158	160	163	rVB	170406	266187	2.83%	0.212%
11	4.030	167	170	173	rBV2	345665	623246	6.62%	0.496%
12	4.098	173	176	179	rBV	312784	585300	6.21%	0.465%
13	4.259	186	190	196	rBV2	1090547	2620803	27.82%	2.084%
14	4.373	196	200	204	rBV2	673904	1107967	11.76%	0.881%
15	4.441	204	206	208	rBV	148716	234116	2.48%	0.186%
16	4.476	208	209	212	rVB	165597	213285	2.26%	0.170%
17	4.544	212	215	218	rBV2	251554	530135	5.63%	0.422%
18	4.601	218	220	222	rBV	328711	454914	4.83%	0.362%
19	4.647	222	224	226	rBV2	142903	200419	2.13%	0.159%
20	4.693	226	228	229	rBV2	269587	498126	5.29%	0.396%
21	4.727	229	231	233	rVB	1654001	1936921	20.56%	1.540%
22	4.773	233	235	236	rBV	357676	659980	7.01%	0.525%
23	4.819	236	239	243	rVB3	2116550	3582311	38.02%	2.849%
24	4.887	243	245	247	rBV2	2352115	3515361	37.31%	2.795%
25	4.933	247	249	250	rVV2	659071	894778	9.50%	0.712%
26	5.024	254	257	262	rVB3	856493	1573520	16.70%	1.251%
27	5.104	262	264	266	rBV	2037648	2787491	29.59%	2.217%
28	5.230	271	275	278	rBV2	842580	1477373	15.68%	1.175%
29	5.287	278	280	281	rBV	987184	1367964	14.52%	1.088%
30	5.390	287	289	293	rBV2	3052950	6259213	66.44%	4.977%
31	5.493	295	298	300	rBV	2068636	3412467	36.22%	2.714%
32	5.527	300	301	303	rVB	1164883	1535965	16.30%	1.221%
33	5.596	303	307	310	rVB2	1607826	3557627	37.76%	2.829%
34	5.653	310	312	316	rVB	1146117	1667900	17.70%	1.326%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
Data File : BF091905.D
Acq On : 23 Dec 2016 5:06
Operator : UM/SJ
Sample : H6182-07RE
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-52(6-8)-121916RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	5.756	316	321	323	rBV2	4353740	9286397	98.57%	7.384%
36	5.802	323	325	327	rBV2	1214100	1828079	19.40%	1.454%
37	5.893	330	333	336	rBV2	5204310	8375262	88.90%	6.660%
38	5.962	336	339	340	rBV3	1262964	2237483	23.75%	1.779%
39	5.996	340	342	346	rVV2	5051946	9421312	100.00%	7.492%
40	6.053	346	347	353	rVB3	2416470	5350572	56.79%	4.255%
41	6.190	356	359	364	rBV4	2156067	6198584	65.79%	4.929%
42	6.282	364	367	372	rBV5	3064246	8293441	88.03%	6.595%
43	6.453	376	382	384	rBV4	2945789	8763110	93.01%	6.968%
44	6.544	388	390	394	rVB2	1489571	2747998	29.17%	2.185%
45	6.613	394	396	397	rBV	987923	996744	10.58%	0.793%
46	6.727	401	406	407	rBV3	1814830	4531193	48.10%	3.603%
47	6.784	409	411	413	rBV	2588151	2823342	29.97%	2.245%
48	6.922	421	423	428	rVB3	1610725	4064029	43.14%	3.232%
49	7.116	438	440	442	rBV2	1090981	1482773	15.74%	1.179%
50	7.162	442	444	445	rBV2	2413762	3360461	35.67%	2.672%


Sum of corrected areas: 125757314

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122216\
Data File : BF091905.D
Acq On : 23 Dec 2016 5:06
Operator : UM/SJ
Sample : H6182-07RE
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-52(6-8)-121916RE

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

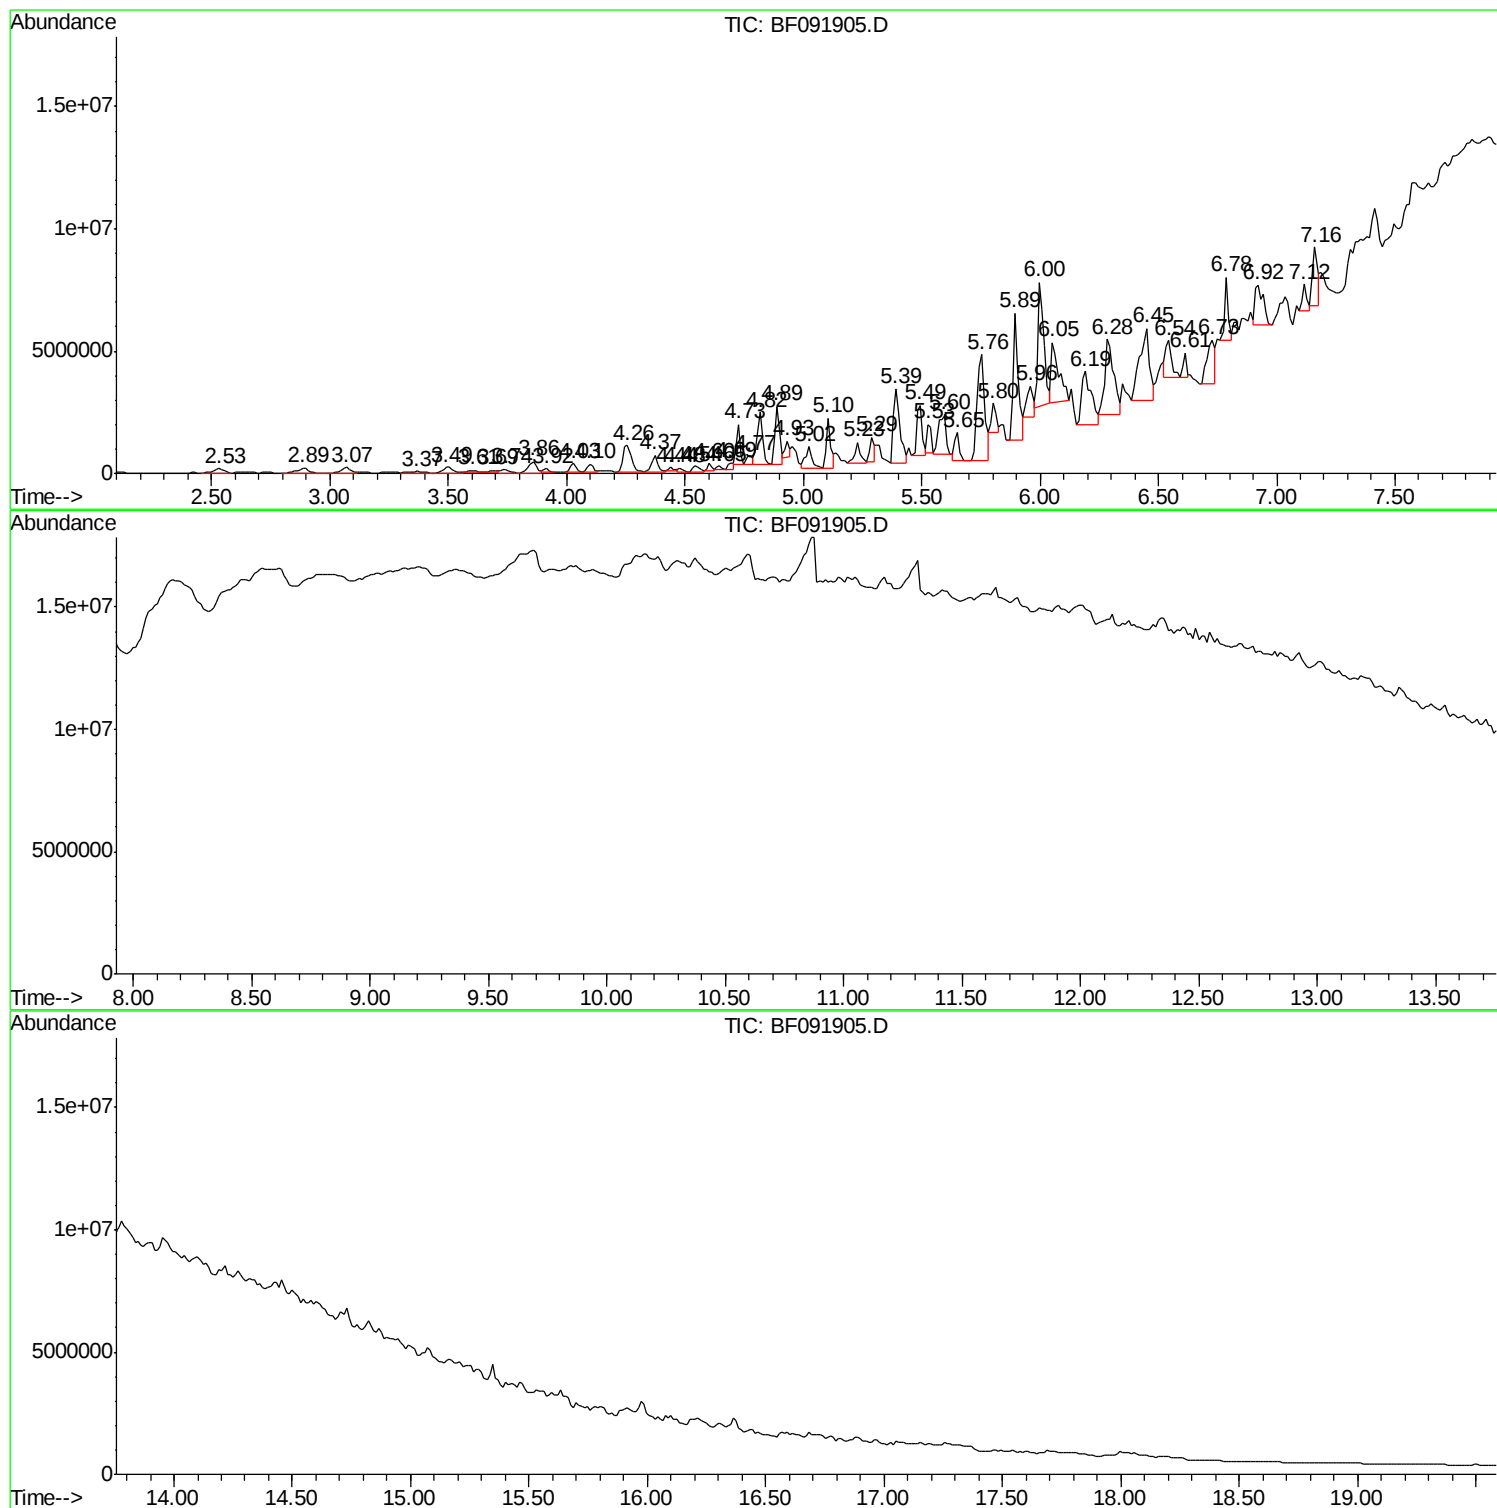

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
Data_File : BF091905.D
Acq_On : 23-Dec-2016 5:066
Operator : UM/SJJ
Sample : H6182-07REE
Misc :
ALS_Vial : 56 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-52(6-8)-121916RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
