

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122216\
 Data File : BF091906.D
 Acq On : 23 Dec 2016 5:33
 Operator : UM/SJ
 Sample : H6182-08RE
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-52(13-15)-121916RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.927	154	161	164	rBV	204037	390275	1.36%	0.104%
2	4.304	190	194	199	rVB2	207408	411048	1.43%	0.110%
3	4.750	228	233	235	rBV	722034	970453	3.38%	0.259%
4	4.841	235	241	245	rBV2	1183553	2260962	7.88%	0.602%
5	4.933	245	249	252	rBV2	1638671	4100511	14.29%	1.093%
6	5.047	255	259	263	rVB2	248783	395267	1.38%	0.105%
7	5.127	263	266	267	rBV	1154828	1705934	5.94%	0.455%
8	5.150	267	268	275	rVB3	325591	735217	2.56%	0.196%
9	5.299	278	281	283	rBV2	229376	356710	1.24%	0.095%
10	5.402	287	290	294	rVB	5083610	6316355	22.00%	1.683%
11	5.493	296	298	301	rBV	1417489	2219671	7.73%	0.591%
12	5.539	301	302	304	rVB	1693356	1742338	6.07%	0.464%
13	5.584	304	306	310	rVB2	1487046	2266865	7.90%	0.604%
14	5.653	310	312	315	rBV	544621	702299	2.45%	0.187%
15	5.756	317	321	323	rBV2	2358140	3690044	12.86%	0.983%
16	5.802	323	325	327	rBV	938077	1713785	5.97%	0.457%
17	5.847	327	329	330	rVB2	285268	342010	1.19%	0.091%
18	5.893	330	333	336	rVB2	3474071	5212957	18.16%	1.389%
19	5.962	336	339	340	rBV2	1349073	2616714	9.12%	0.697%
20	5.996	340	342	346	rBV2	5423681	9668657	33.68%	2.576%
21	6.053	346	347	349	rBV	1803910	2651808	9.24%	0.707%
22	6.190	356	359	365	rBV4	2577656	6854718	23.88%	1.827%
23	6.282	365	367	372	rBV2	3914073	9102681	31.71%	2.426%
24	6.373	372	375	376	rBV2	998334	2173987	7.57%	0.579%
25	6.453	376	382	384	rVV3	4785410	10117339	35.25%	2.696%
26	6.510	384	387	388	rBV	3275407	7344781	25.59%	1.957%
27	6.545	388	390	393	rVB	5193518	8336839	29.04%	2.222%
28	6.613	393	396	398	rBV3	1813932	3097141	10.79%	0.825%
29	6.727	401	406	407	rBV3	2519067	7111557	24.77%	1.895%
30	6.762	407	409	413	rVB4	2410810	6073300	21.16%	1.618%
31	6.830	413	415	417	rBV	1525868	3368256	11.73%	0.898%
32	6.922	419	423	428	rVB4	7554685	19279779	67.17%	5.137%
33	7.036	428	433	437	rBV3	2983834	9817325	34.20%	2.616%
34	7.127	439	441	442	rBV2	836436	1591093	5.54%	0.424%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
 Data File : BF091906.D
 Acq On : 23 Dec 2016 5:33
 Operator : UM/SJ
 Sample : H6182-08RE
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-52(13-15)-121916RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	7.162	442	444	450	rVB4	3315350	8844830	30.81%	2.357%
36	7.322	453	458	464	rBV6	7159296	28704967	100.00%	7.649%
37	7.425	464	467	470	rVB2	3406892	7016508	24.44%	1.870%
38	7.585	476	481	484	rVB5	4080695	12724076	44.33%	3.391%
39	7.699	487	491	498	rVV5	5176717	16988354	59.18%	4.527%
40	7.813	498	501	506	rVB2	3723828	9599048	33.44%	2.558%
41	7.905	506	509	510	rBV3	1824508	3600782	12.54%	0.959%
42	8.282	537	542	546	rBV7	2789026	11822349	41.19%	3.150%
43	8.373	547	550	552	rVB5	3113784	7032125	24.50%	1.874%
44	8.522	560	563	567	rBV2	5099109	11779790	41.04%	3.139%
45	8.590	567	569	571	rBV2	1721721	1996168	6.95%	0.532%
46	9.116	612	615	616	rBV2	5408911	7701119	26.83%	2.052%
47	9.253	623	627	628	rBV2	2787924	6501929	22.65%	1.733%
48	9.425	640	642	644	rVB	3451745	4078830	14.21%	1.087%
49	9.493	646	648	649	rVV	3381881	4752088	16.55%	1.266%
50	9.562	651	654	655	rVB2	5944080	8653009	30.14%	2.306%
51	9.733	667	669	671	rVB2	2394237	2524956	8.80%	0.673%
52	9.813	673	676	678	rVV3	2433880	5802554	20.21%	1.546%
53	9.859	678	680	681	rVV2	2377294	2777340	9.68%	0.740%
54	9.928	684	686	688	rVB	3012187	3893647	13.56%	1.038%
55	9.962	688	689	692	rBV3	1340107	3093043	10.78%	0.824%
56	10.019	692	694	696	rVB2	2832893	4063929	14.16%	1.083%
57	10.076	696	699	702	rVB3	3577297	7238134	25.22%	1.929%
58	10.133	702	704	705	rBV	2673688	2877726	10.03%	0.767%
59	10.225	710	712	714	rVB2	1763527	3029294	10.55%	0.807%
60	10.271	714	716	717	rBV2	972901	1312269	4.57%	0.350%
61	10.351	721	723	726	rBV3	1621342	3277191	11.42%	0.873%
62	10.465	730	733	735	rVB	3826359	5808552	20.24%	1.548%
63	10.499	735	736	739	rVB3	1128692	1609137	5.61%	0.429%
64	10.568	741	742	743	rVB	877390	601890	2.10%	0.160%
65	10.591	743	744	746	rVB	1683322	1500885	5.23%	0.400%
66	10.716	753	755	758	rVB	4195121	6040448	21.04%	1.610%
67	10.922	771	773	776	rVB4	583895	917208	3.20%	0.244%
68	11.036	781	783	789	rVB5	541330	1063682	3.71%	0.283%
69	11.174	793	795	798	rVB	1365179	1723948	6.01%	0.459%
70	11.276	802	804	808	rBV2	1074401	1329249	4.63%	0.354%
71	11.528	824	826	828	rVV2	447030	625048	2.18%	0.167%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
 Data File : BF091906.D
 Acq On : 23 Dec 2016 5:33
 Operator : UM/SJ
 Sample : H6182-08RE
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-52(13-15)-121916RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.562	828	829	831	rVB2	286985	354111	1.23%	0.094%
73	11.665	836	838	840	rBV	793012	672969	2.34%	0.179%
74	11.768	845	847	849	rBV3	347846	618313	2.15%	0.165%
75	11.814	849	851	853	rVV3	278090	465766	1.62%	0.124%
76	11.859	853	855	856	rVV	898854	1008590	3.51%	0.269%
77	11.894	856	858	862	rVB4	443804	710641	2.48%	0.189%
78	11.962	862	864	867	rBV2	579069	881616	3.07%	0.235%
79	12.019	867	869	870	rVV	358030	667332	2.32%	0.178%
80	12.054	870	872	875	rVV	1433781	1638802	5.71%	0.437%
81	12.122	875	878	883	rVB4	493223	962712	3.35%	0.257%
82	12.214	883	886	888	rBV2	590296	754075	2.63%	0.201%
83	12.294	891	893	899	rVV	1219482	1601542	5.58%	0.427%
84	12.397	900	902	904	rVB	299796	351799	1.23%	0.094%
85	12.522	910	913	915	rVB2	560266	587643	2.05%	0.157%
86	12.819	937	939	940	rBV	639801	570030	1.99%	0.152%
87	12.854	940	942	945	rVB	3348378	3480169	12.12%	0.927%
88	12.991	952	954	956	rVB	303738	293909	1.02%	0.078%
89	13.334	982	984	987	rVB	283452	446816	1.56%	0.119%
90	13.905	1031	1034	1036	rVB	587383	833512	2.90%	0.222%
91	15.300	1153	1156	1161	rVB	536930	734055	2.56%	0.196%


Sum of corrected areas: 375279180

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
Data File : BF091906.D
Acq On : 23 Dec 2016 5:33
Operator : UM/SJ
Sample : H6182-08RE
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-52(13-15)-121916RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

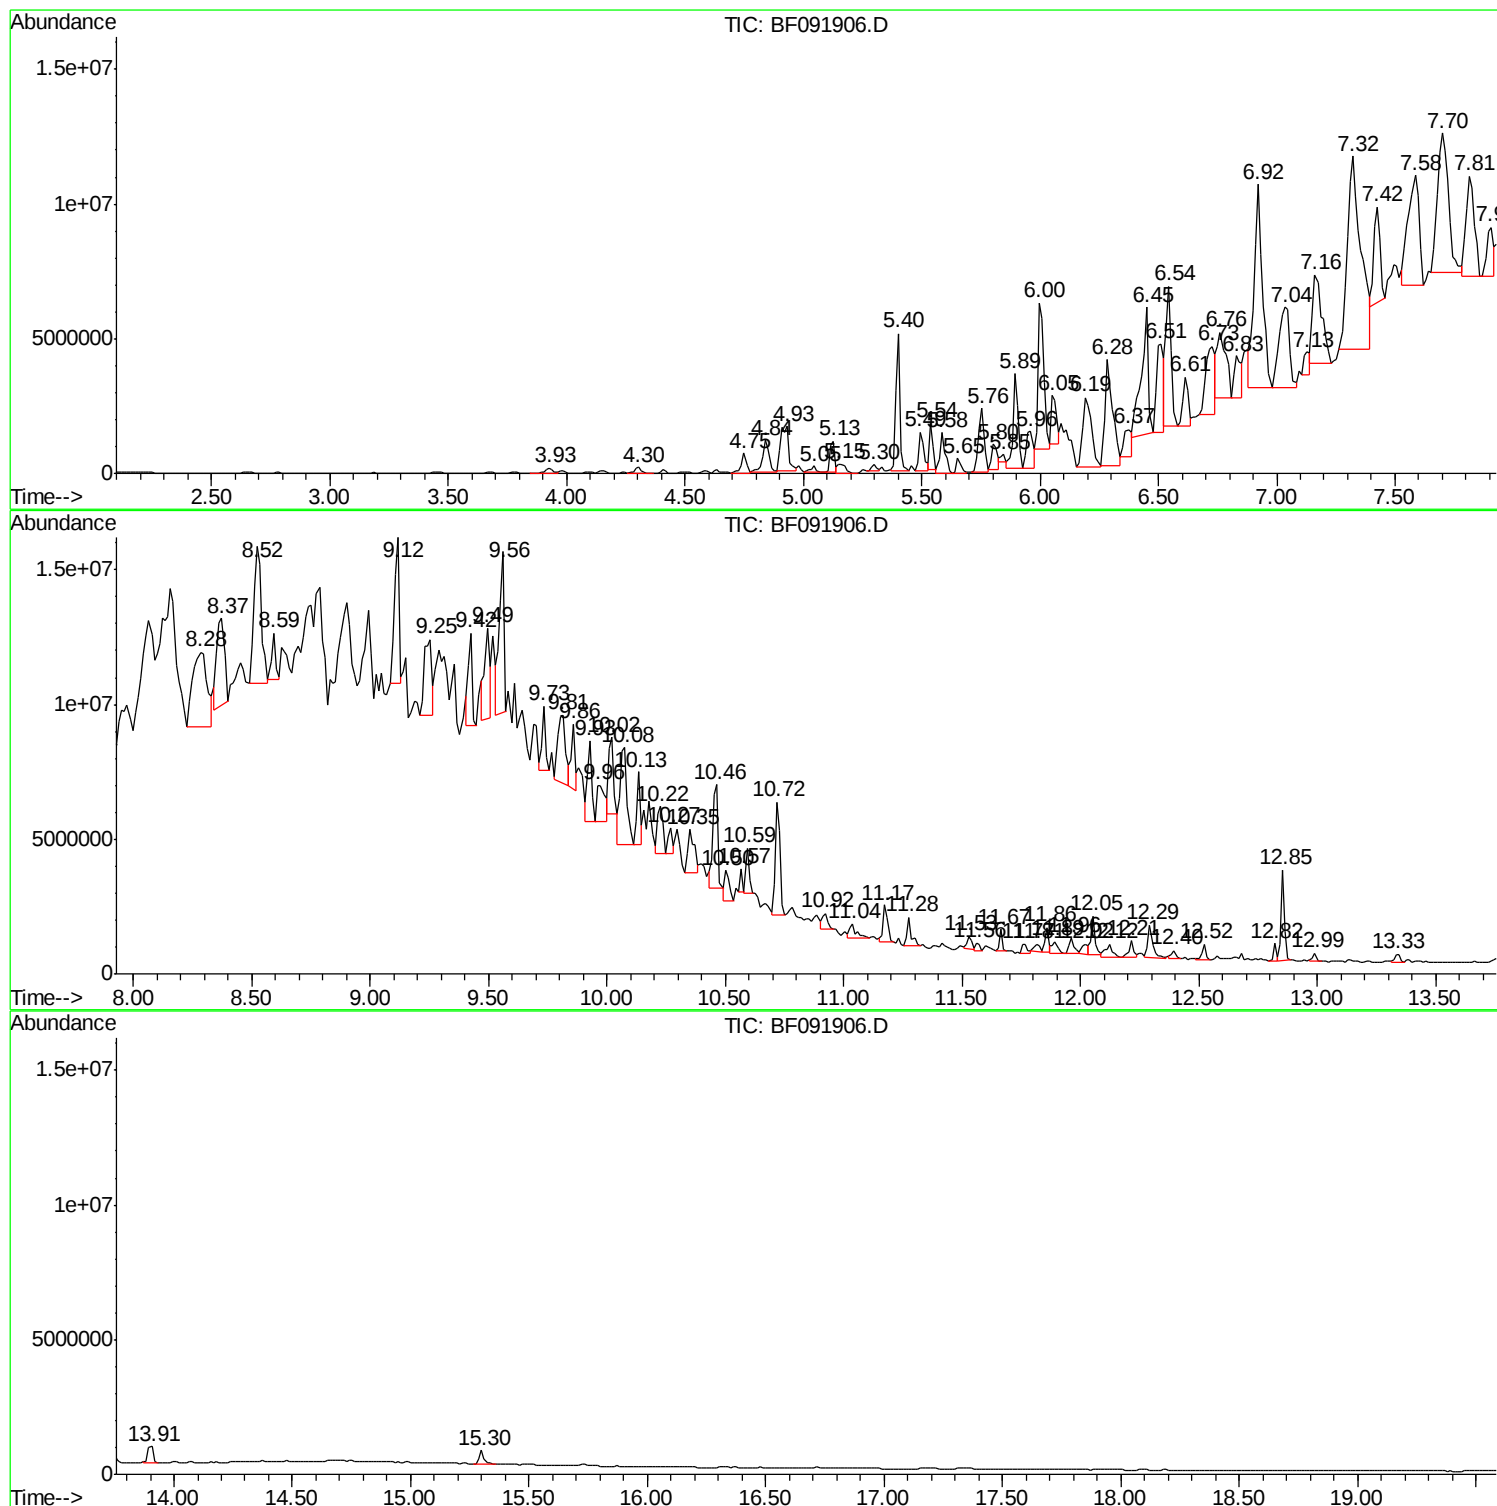

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
Data_File : BF091906.D
Acq_On : 23-Dec-2016 5:333
Operator : UM/SJJ
Sample : H6182-08REE
Misc :
ALS_Vial : 57 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-52(13-15)-121916RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
