


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122216\
 Data File : BF091900.D
 Acq On : 23 Dec 2016 1:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 16:17:51 2016

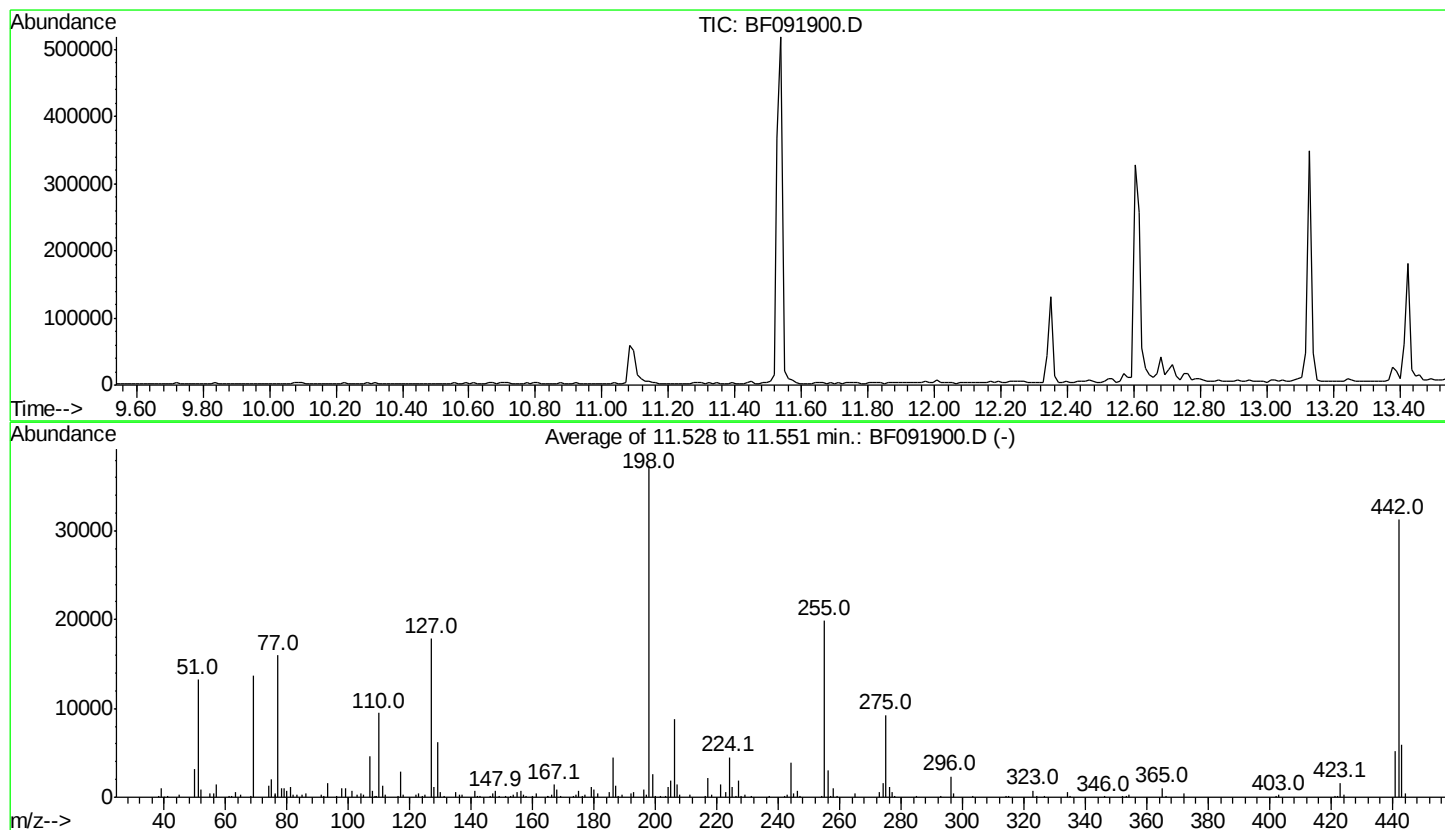

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	13209	PASS
68	69	0.00	2	1.4	188	PASS
69	198	0.00	100	36.6	13665	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	17832	PASS
197	198	0.00	2	0.8	285	PASS
198	198	100	100	100.0	37355	PASS
199	198	5	9	6.8	2550	PASS
275	198	10	60	24.9	9294	PASS
365	198	1	100	2.8	1059	PASS
441	442	0.01	24	16.6	5170	PASS
442	198	50	100	83.6	31237	PASS
443	442	15	24	19.0	5924	PASS