
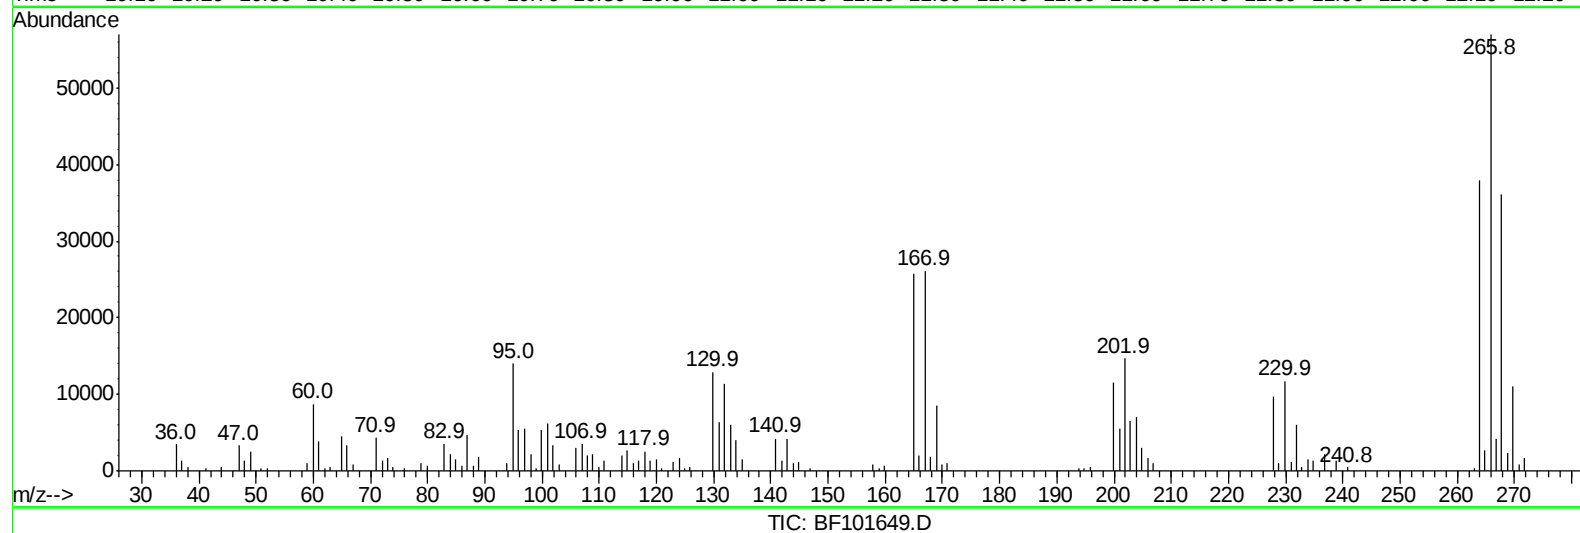


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122217\
Data File : BF101649.D
Acq On : 22 Dec 2017 12:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 03:46:39 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 16:07:58 2017
Response via : Initial Calibration

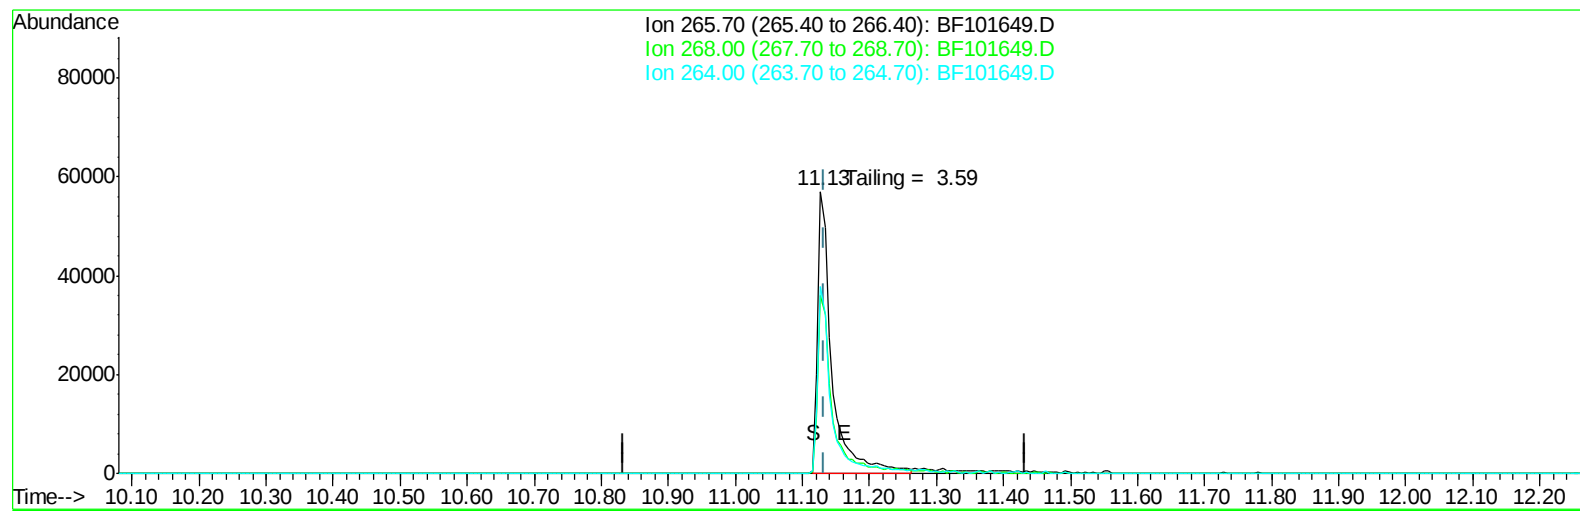

(69) Pentachlorophenol (C)

11.127min (-0.006) 40543.10ng

response 81680

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.25
264.00	61.90	66.46
0.00	0.00	0.00