
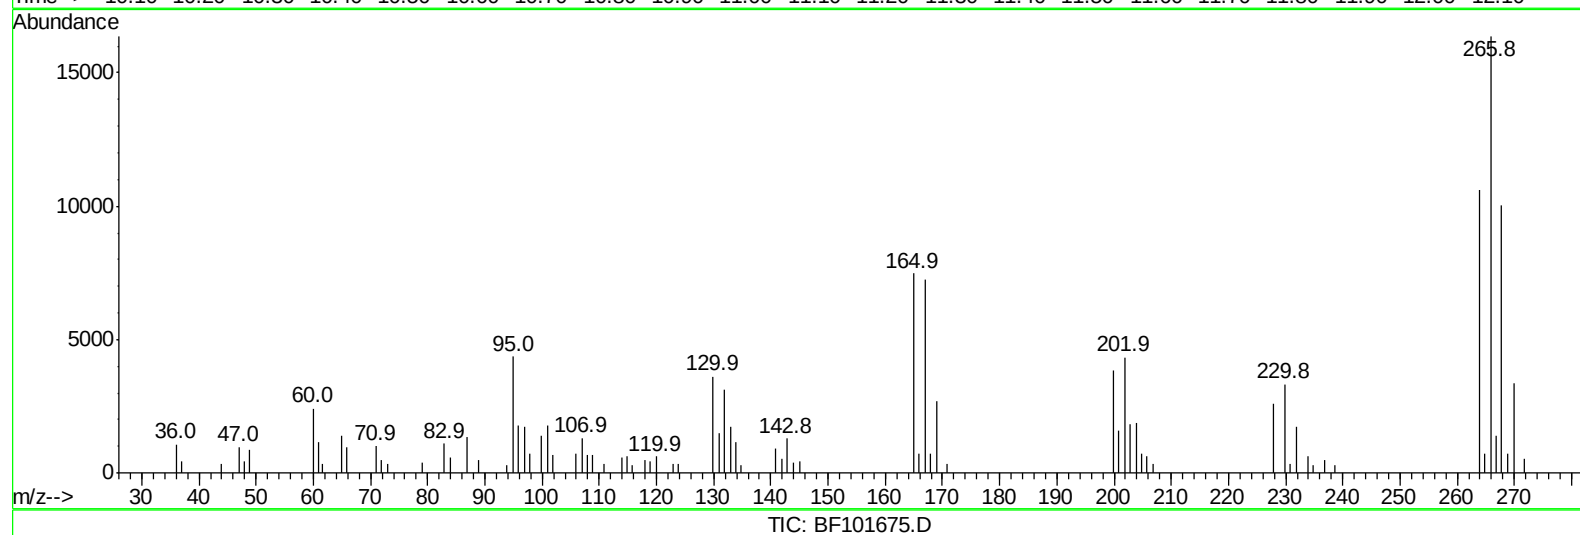


Data Path : Z:\HPCHEM1\BNA F\DATA\BF122217\
Data File : BF101675.D
Acq On : 23 Dec 2017 1:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 03:47:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 16:07:58 2017
Response via : Initial Calibration

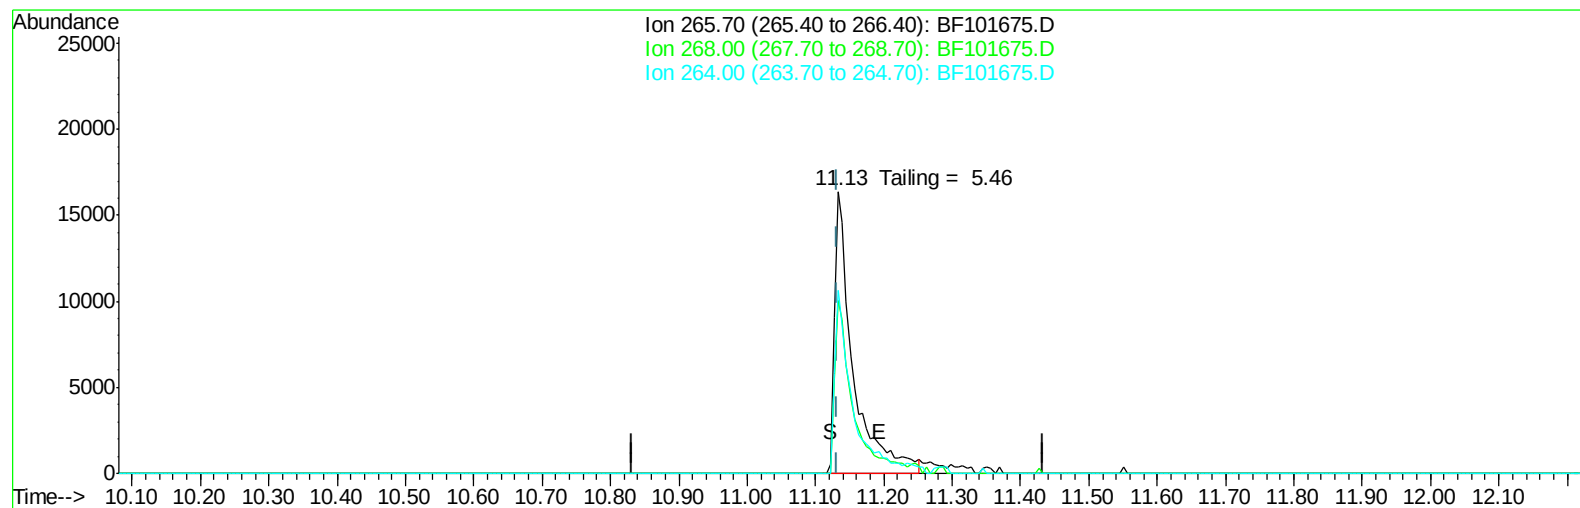

(69) Pentachlorophenol (C)



11.133min (+0.000) 19913.51ng

response 29382

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.32
264.00	61.90	64.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF122217\
Data File : BF101675.D
Acq On : 23 Dec 2017 1:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 03:47:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 16:07:58 2017
Response via : Initial Calibration

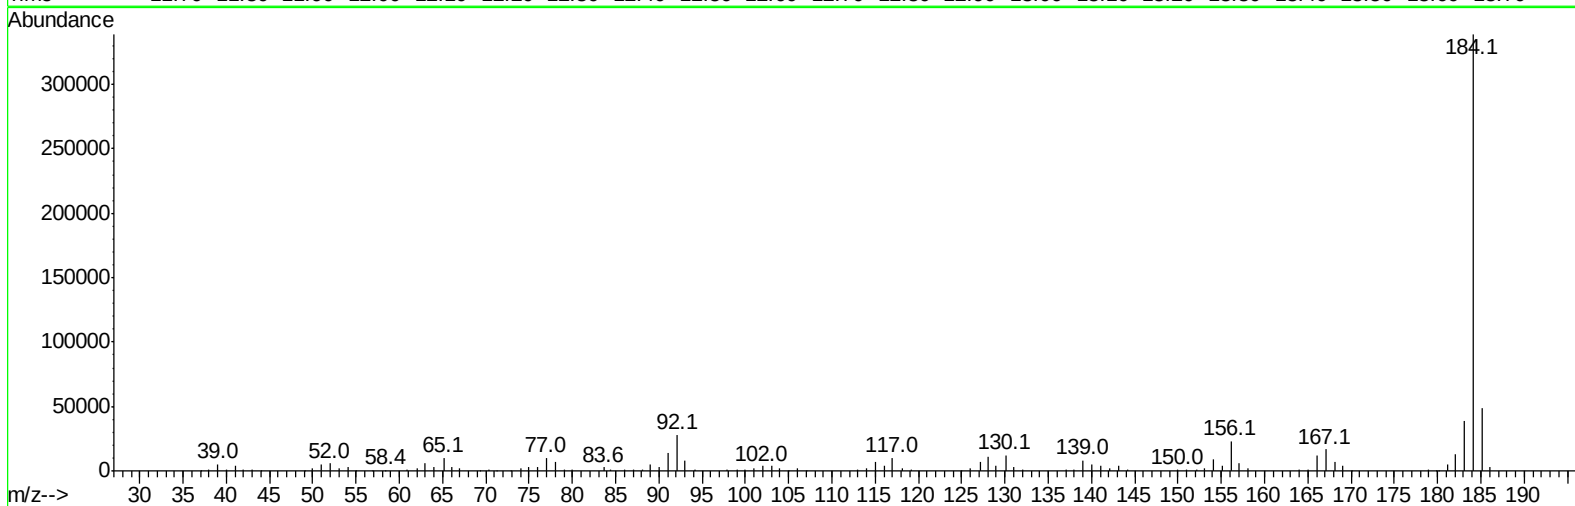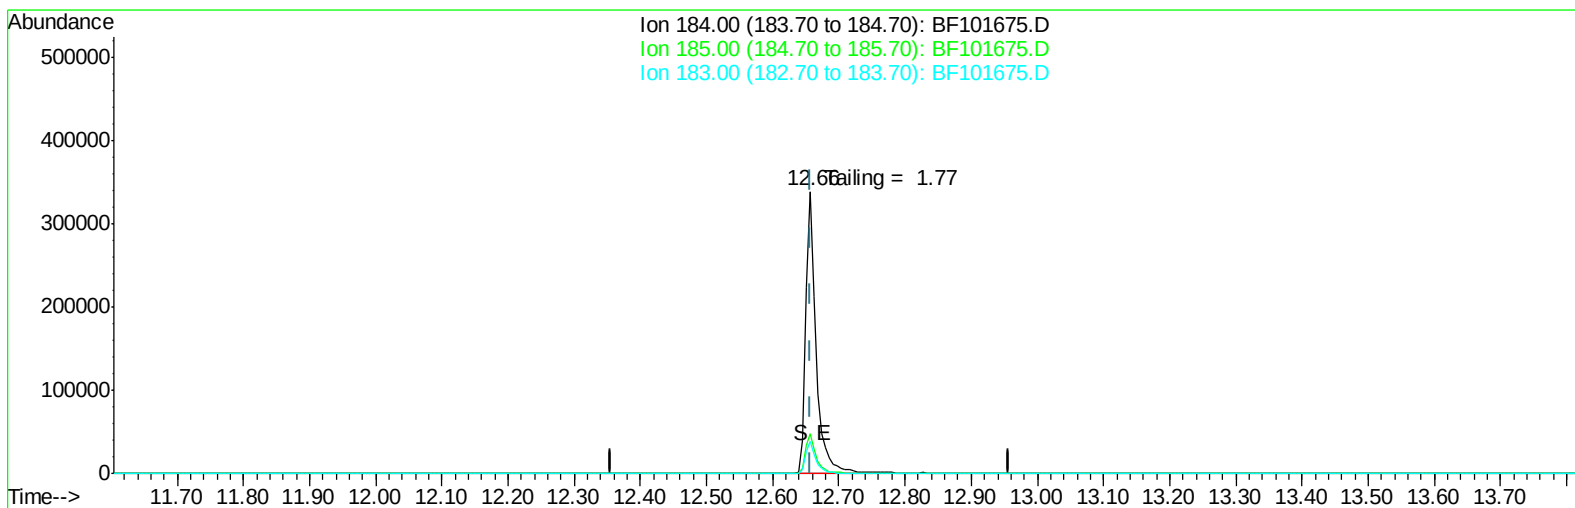

TIC: BF101675.D

(76) Benzidine

12.657min (+0.000) 0.00ng

response 376498

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.29
183.00	11.60	11.44
0.00	0.00	0.00