

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
 Data File : BF101668.D
 Acq On : 22 Dec 2017 21:56
 Operator : SJ/JU
 Sample : I6677-11 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-122117-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.998	492	495	506	rBV	19479	39540	3.64%	0.437%
2	5.422	564	567	591	rBV	110547	271774	25.01%	3.001%
3	6.445	738	741	759	rBV	129888	291484	26.82%	3.219%
4	6.569	759	762	772	rVB	238078	310188	28.54%	3.425%
5	6.786	796	799	811	rBV	866843	833991	76.73%	9.210%
6	6.945	822	826	840	rBV	211362	246164	22.65%	2.718%
7	7.369	894	898	915	rBV	89923	187834	17.28%	2.074%
8	8.069	1014	1017	1036	rBV	1120909	1086864	100.00%	12.002%
9	8.798	1138	1141	1148	rBV	9381	14305	1.32%	0.158%
10	8.886	1154	1156	1161	rBV2	9465	10963	1.01%	0.121%
11	9.139	1196	1199	1208	rBV	343933	338944	31.19%	3.743%
12	9.210	1208	1211	1214	rVB2	11605	11882	1.09%	0.131%
13	9.545	1266	1268	1274	rVB	14260	14747	1.36%	0.163%
14	9.692	1287	1293	1296	rBV	12628	15103	1.39%	0.167%
15	9.739	1299	1301	1305	rVB	17321	14763	1.36%	0.163%
16	9.822	1312	1315	1319	rBV2	1116496	998302	91.85%	11.024%
17	9.857	1319	1321	1327	rVB	38317	39028	3.59%	0.431%
18	10.039	1348	1352	1354	rBV2	10343	12504	1.15%	0.138%
19	10.239	1383	1386	1389	rVB	21192	16597	1.53%	0.183%
20	10.380	1406	1410	1416	rVB2	28389	31864	2.93%	0.352%
21	10.457	1416	1423	1427	rVB5	8571	13741	1.26%	0.152%
22	10.621	1448	1451	1463	rVB	108439	134037	12.33%	1.480%
23	10.710	1463	1466	1472	rVB	18606	22349	2.06%	0.247%
24	11.157	1540	1542	1545	rBV2	13639	12143	1.12%	0.134%
25	11.316	1565	1569	1571	rBV	1015237	887866	81.69%	9.805%
26	11.339	1571	1573	1578	rVV	181272	166740	15.34%	1.841%
27	11.398	1580	1583	1586	rVB	38720	35506	3.27%	0.392%
28	11.821	1651	1655	1657	rBV	17070	17299	1.59%	0.191%
29	11.851	1657	1660	1663	rVB	17106	17851	1.64%	0.197%
30	11.933	1670	1674	1677	rBV	28537	30825	2.84%	0.340%
31	12.374	1745	1749	1751	rBV4	32221	41287	3.80%	0.456%
32	12.392	1751	1752	1757	rVB4	13768	15722	1.45%	0.174%
33	12.533	1772	1776	1781	rBV	184378	161928	14.90%	1.788%
34	12.762	1809	1815	1821	rBV	150944	175353	16.13%	1.936%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
Data File : BF101668.D
Acq On : 22 Dec 2017 21:56
Operator : SJ/JU
Sample : I6677-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-122117-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.815	1821	1824	1830	rBV5	8862	12348	1.14%	0.136%
36	12.892	1834	1837	1841	rBV	312203	261471	24.06%	2.887%
37	12.980	1848	1852	1858	rBV5	12823	27606	2.54%	0.305%
38	13.074	1864	1868	1869	rBV4	9954	14334	1.32%	0.158%
39	13.092	1869	1871	1876	rVB	24134	28104	2.59%	0.310%
40	13.162	1880	1883	1885	rVB	20459	18049	1.66%	0.199%
41	13.198	1885	1889	1891	rBV5	15924	20570	1.89%	0.227%
42	13.292	1902	1905	1908	rBV2	15106	16884	1.55%	0.186%
43	13.321	1908	1910	1912	rBV3	15769	14744	1.36%	0.163%
44	13.498	1937	1940	1941	rBV3	11798	10882	1.00%	0.120%
45	13.715	1975	1977	1979	rBV2	15095	16180	1.49%	0.179%
46	13.786	1984	1989	1993	rBV7	21996	45045	4.14%	0.497%
47	13.962	2014	2019	2022	rBV	916380	939531	86.44%	10.375%
48	13.992	2022	2024	2027	rVB	74137	70395	6.48%	0.777%
49	14.074	2035	2038	2040	rBV2	20388	25171	2.32%	0.278%
50	15.009	2194	2197	2207	rVB2	71019	159888	14.71%	1.766%
51	15.368	2256	2258	2264	rVV2	51213	70579	6.49%	0.779%
52	15.427	2264	2268	2278	rVB	602898	784314	72.16%	8.661%


Sum of corrected areas: 9055583

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
Data File : BF101668.D
Acq On : 22 Dec 2017 21:56
Operator : SJ/JU
Sample : I6677-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-122117-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

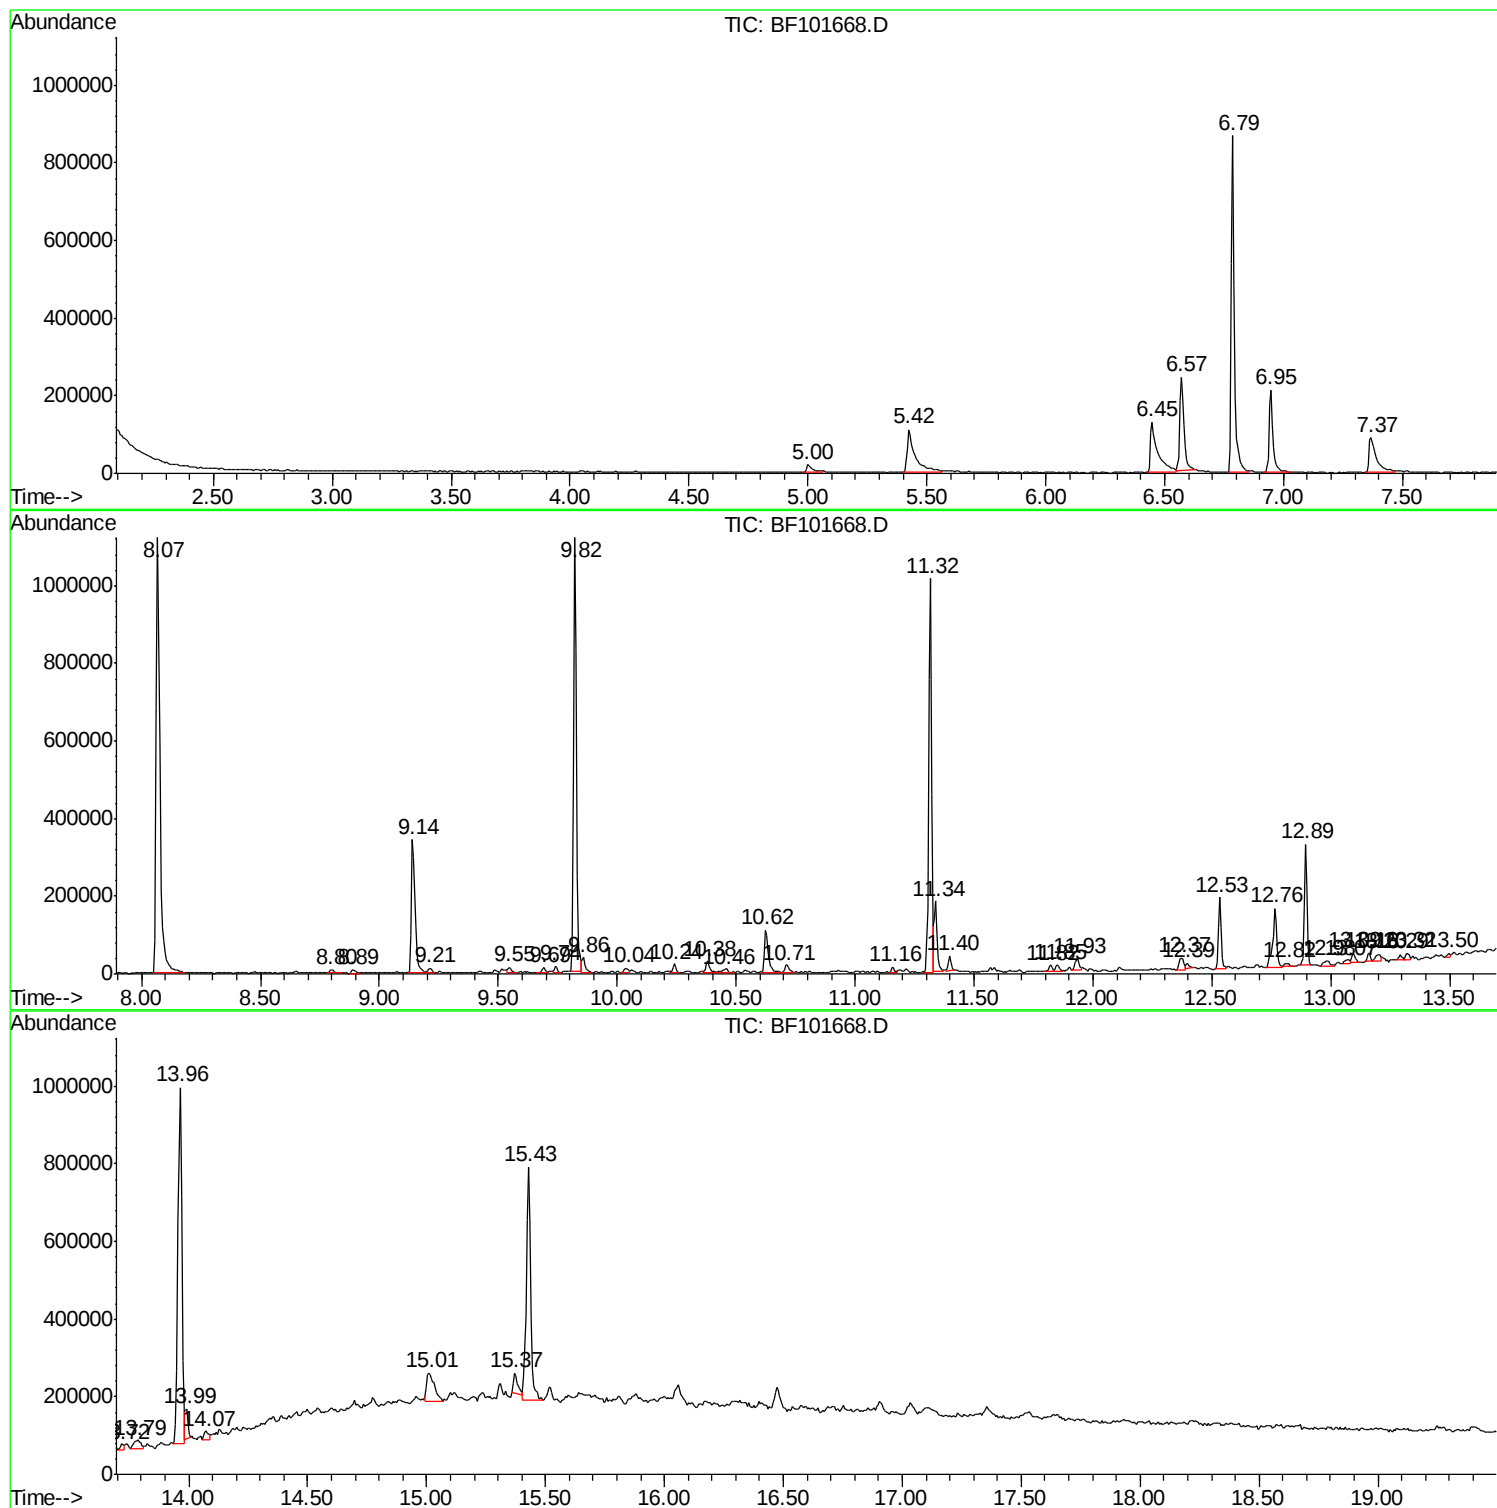

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
Data File : BF101668.D
Acq On : 22 Dec 2017 21:56
Operator : SJ/JU
Sample : I6677-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-122117-B








Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	7.44 ng	310188	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

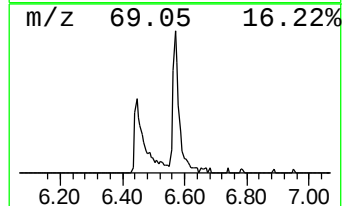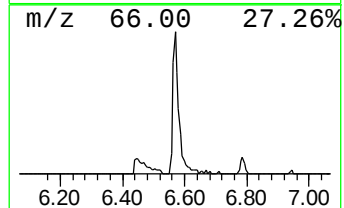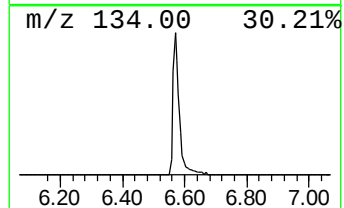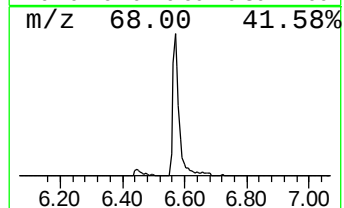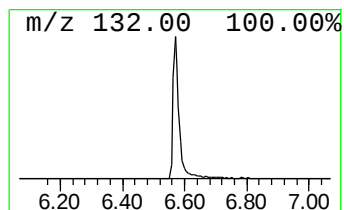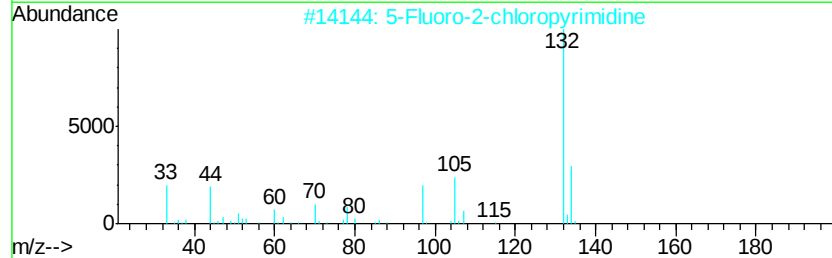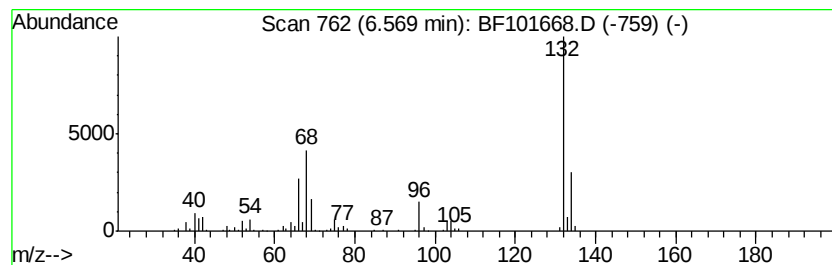

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
Data File : BF101668.D
Acq On : 22 Dec 2017 21:56
Operator : SJ/JU
Sample : I6677-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-122117-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.57	6.57	7.4	ng	310188	1	6.79	833991	20.0