


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
 Data File : BF101649.D
 Acq On : 22 Dec 2017 12:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 16:07:58 2017

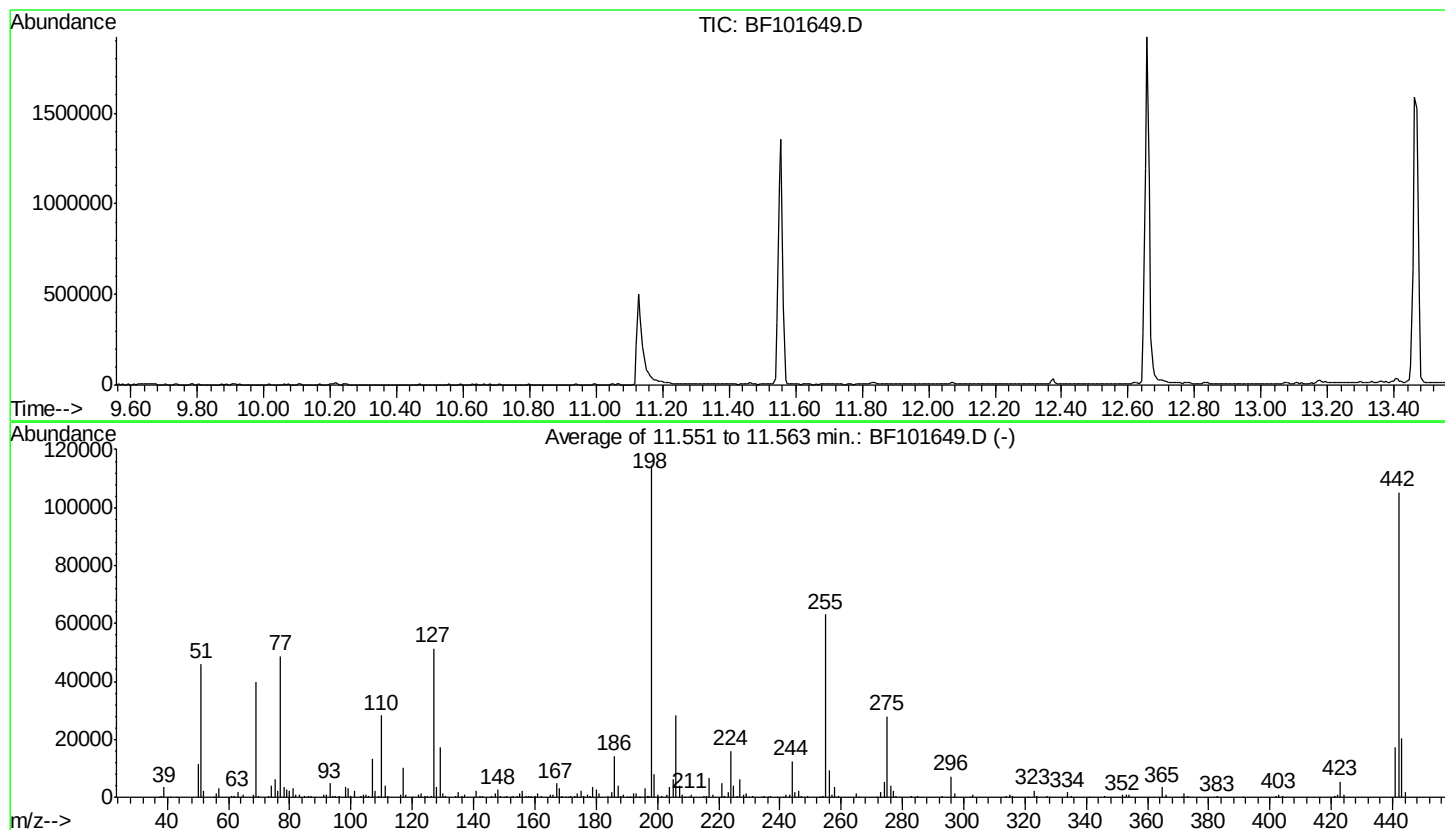

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	46162	PASS
68	69	0.00	2	1.8	703	PASS
69	198	0.00	100	34.9	39914	PASS
70	69	0.00	2	0.7	261	PASS
127	198	10	80	44.9	51370	PASS
197	198	0.00	2	0.6	652	PASS
198	198	100	100	100.0	114474	PASS
199	198	5	9	7.0	7960	PASS
275	198	10	60	24.3	27872	PASS
365	198	1	100	3.0	3474	PASS
441	443	0.01	100	86.0	17377	PASS
442	198	50	100	92.0	105370	PASS
443	442	15	24	19.2	20212	PASS