


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF122217\
 Data File : BF101675.D
 Acq On : 23 Dec 2017 1:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 16:07:58 2017

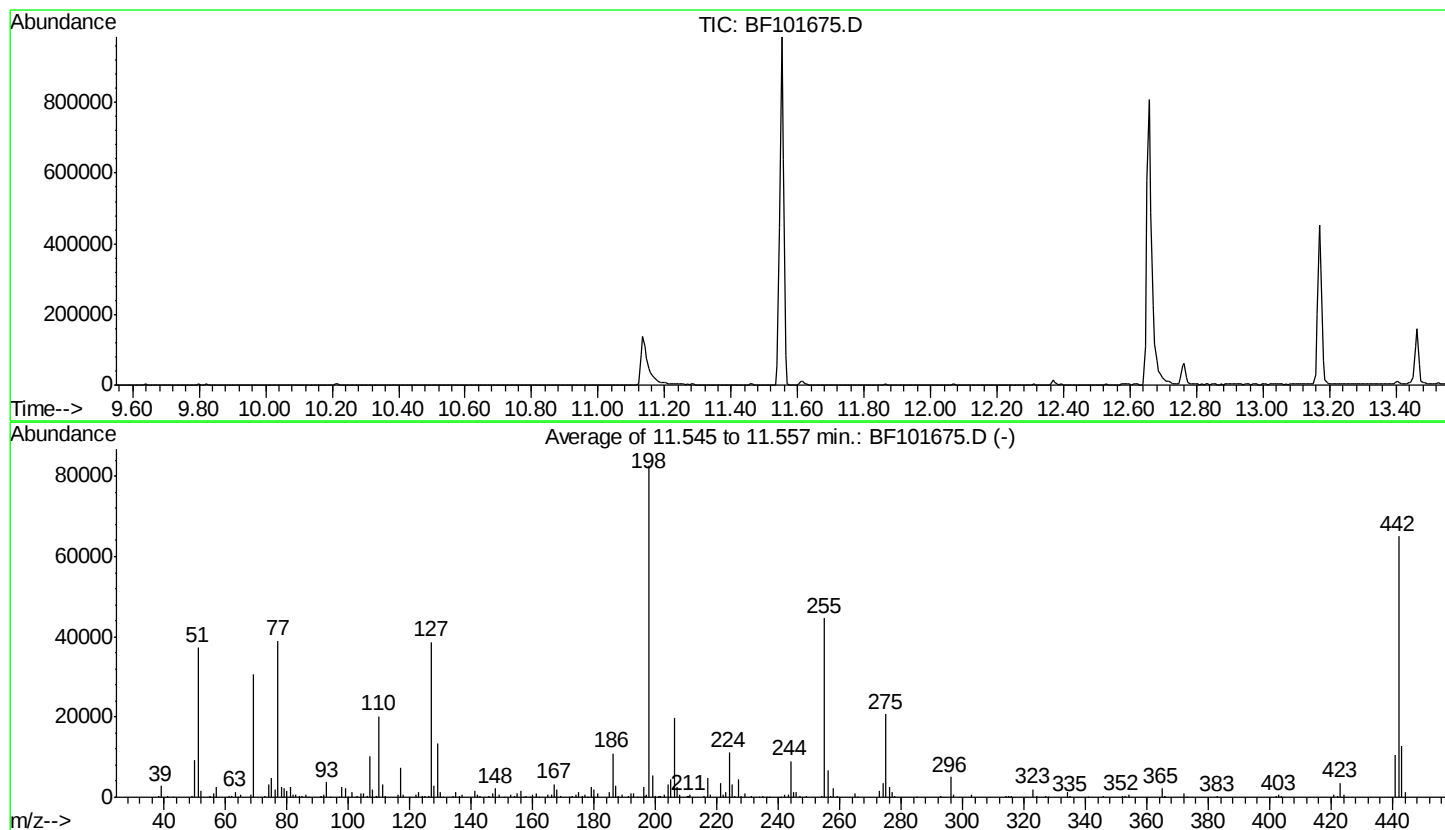

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	37261	PASS
68	69	0.00	2	1.8	549	PASS
69	198	0.00	100	37.0	30549	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	38664	PASS
197	198	0.00	2	0.7	590	PASS
198	198	100	100	100.0	82650	PASS
199	198	5	9	6.7	5554	PASS
275	198	10	60	25.0	20630	PASS
365	198	1	100	2.6	2111	PASS
441	443	0.01	100	83.2	10508	PASS
442	198	50	100	78.6	64997	PASS
443	442	15	24	19.4	12634	PASS