
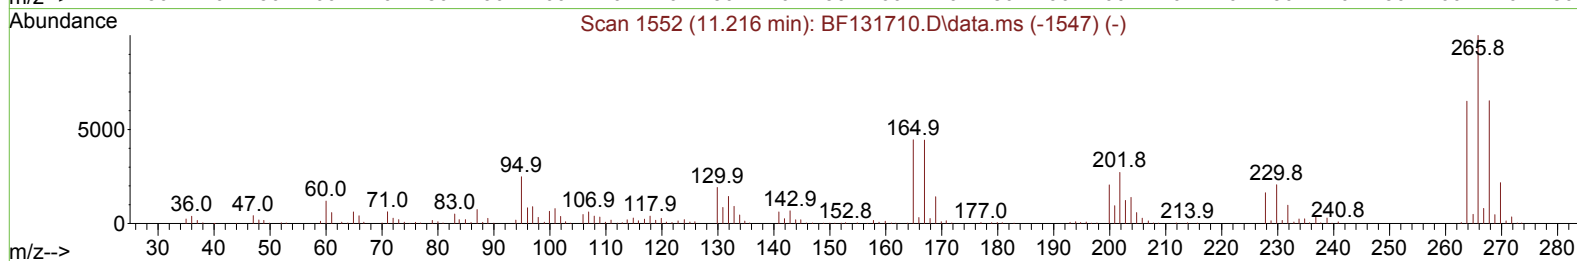
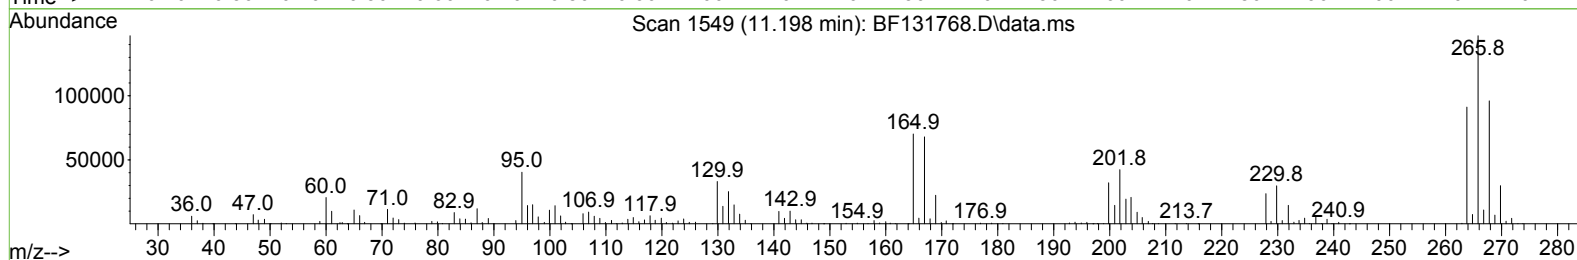


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131768.D
Acq On : 22 Dec 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

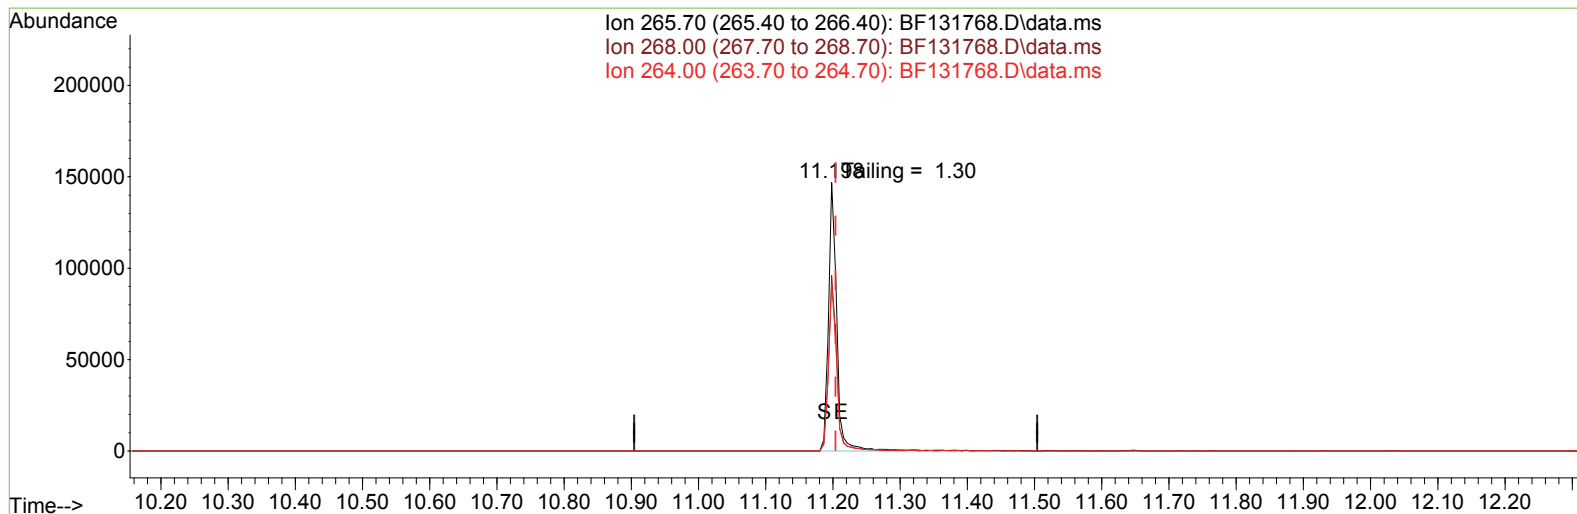

TIC: BF131768.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 31630.88 ng

response 126045

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.40
264.00	65.00	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131768.D
Acq On : 22 Dec 2022 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

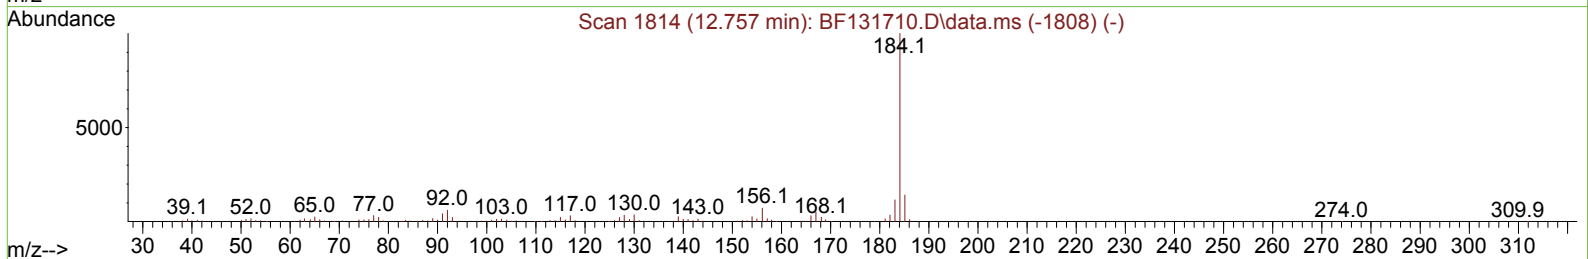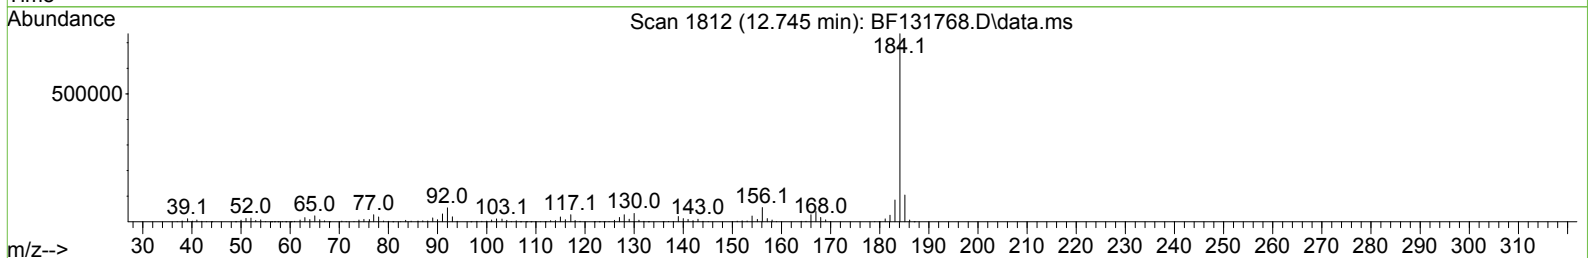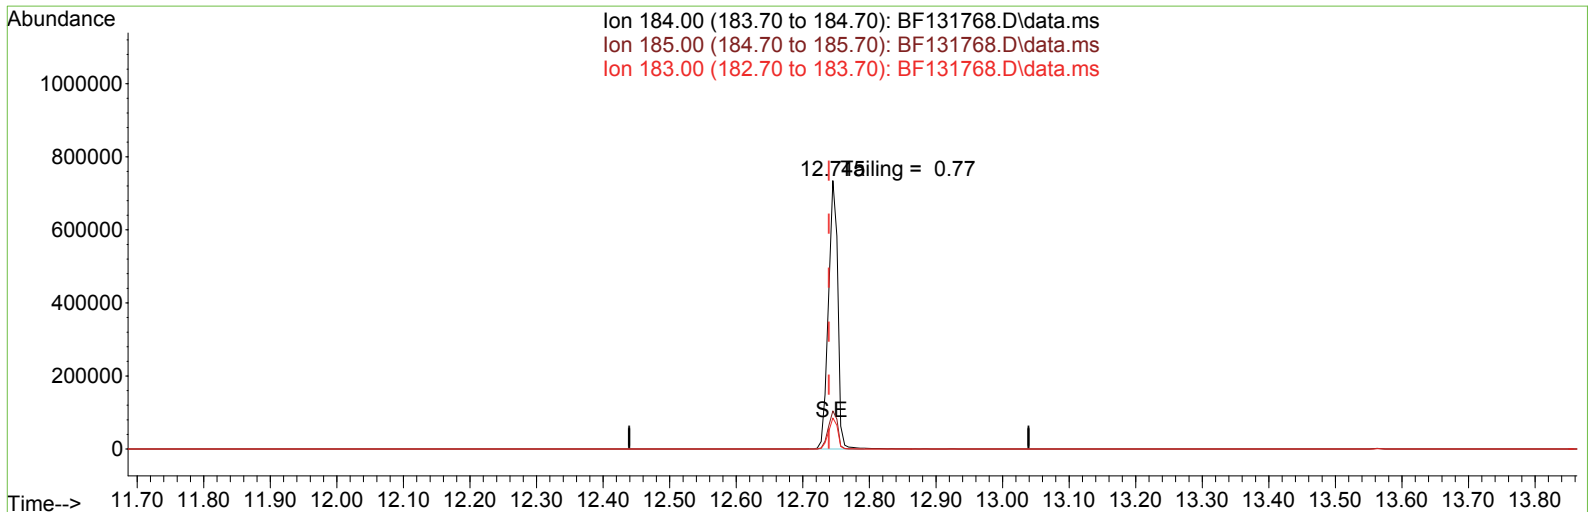

TIC: BF131768.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng

response 720501

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.20
183.00	11.60	11.58
0.00	0.00	0.00