
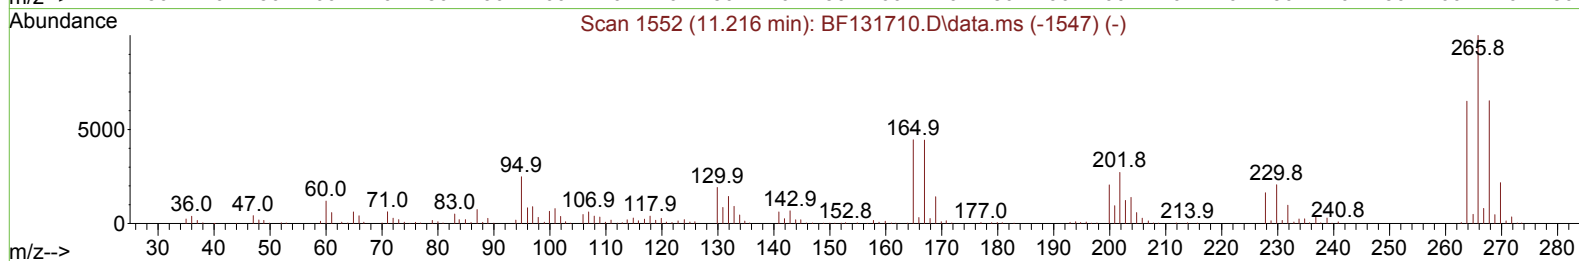
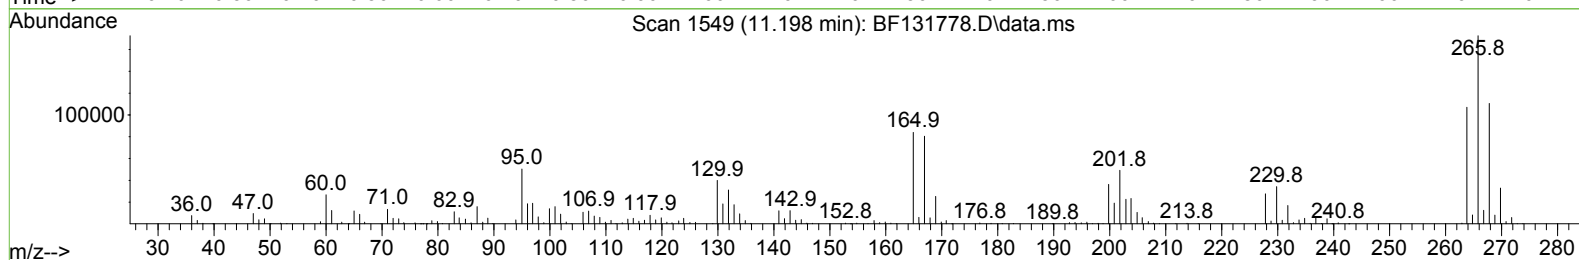


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131778.D
Acq On : 22 Dec 2022 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

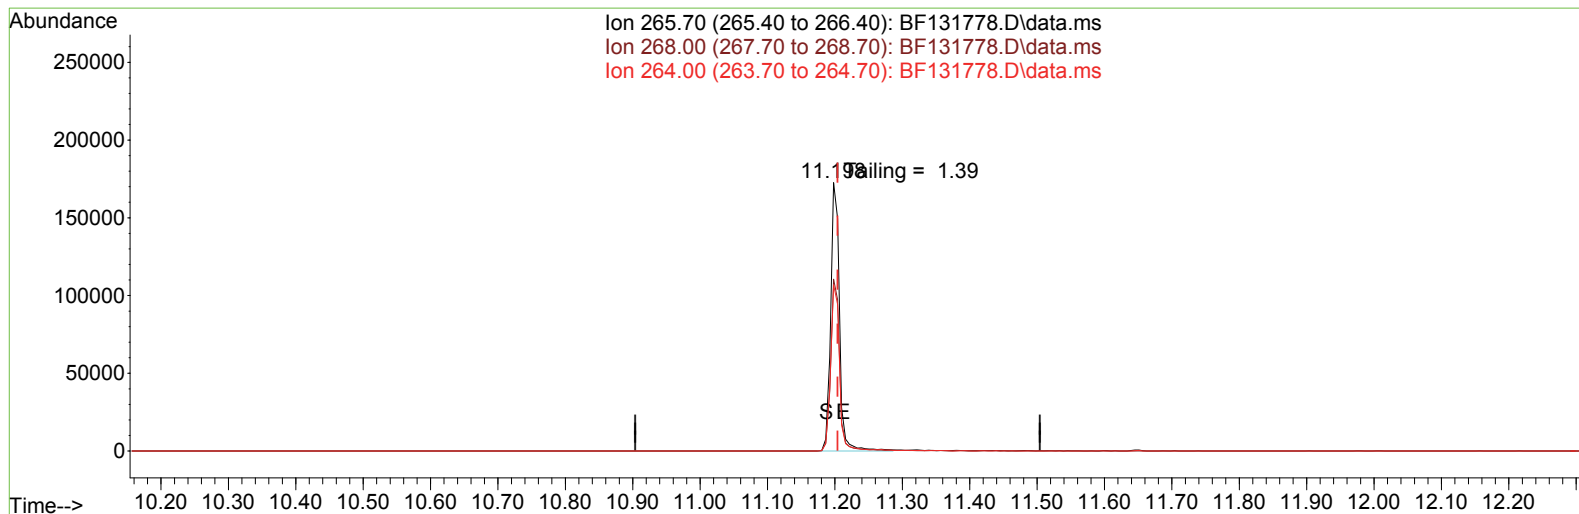

TIC: BF131778.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 27000.22 ng

response 158038

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.02
264.00	65.00	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131778.D
Acq On : 22 Dec 2022 15:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 05:57:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 03:03:57 2022
Response via : Initial Calibration

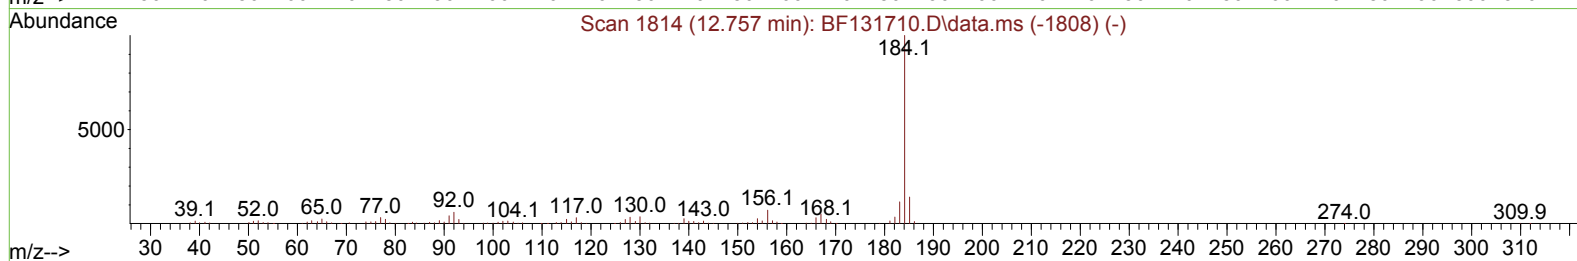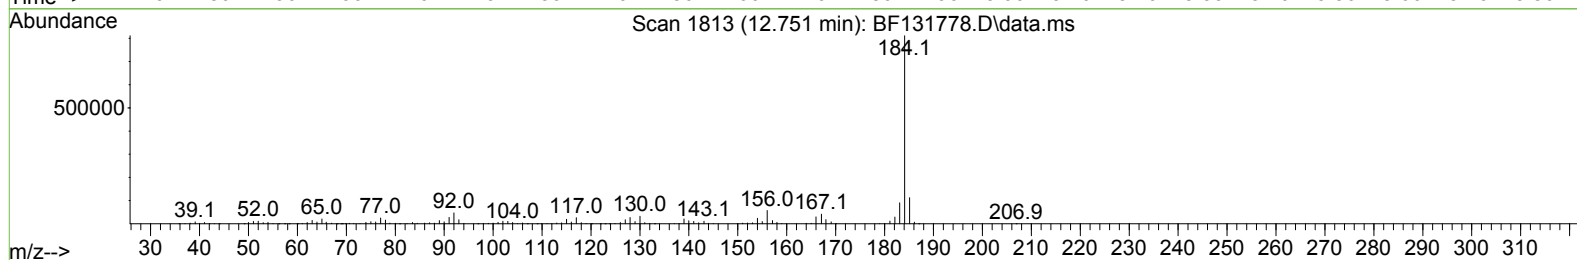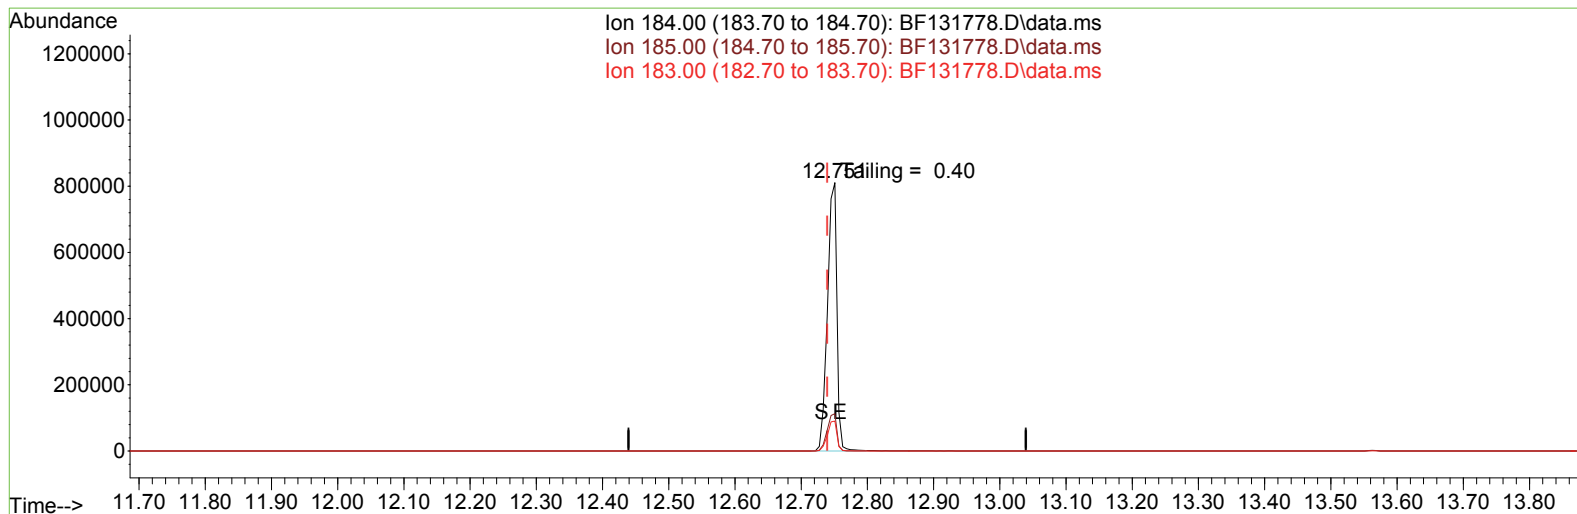

TIC: BF131778.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 0.00 ng

response 805819

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.90
183.00	11.60	11.20
0.00	0.00	0.00