

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
 Data File : BF131776.D
 Acq On : 22 Dec 2022 14:37
 Operator : CG\JU
 Sample : N6102-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-7

Quant Time: Dec 23 01:53:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 01:24:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.851	152	80191	20.000	ng	0.00
21) Naphthalene-d8	8.139	136	295736	20.000	ng	0.00
39) Acenaphthene-d10	9.904	164	169156	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	340542	20.000	ng	0.00
76) Chrysene-d12	14.045	240	229809	20.000	ng	0.00
86) Perylene-d12	15.533	264	183757	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.463	112	319560	67.103	ng	0.00
7) Phenol-d6	6.481	99	275170	42.929	ng	0.00
23) Nitrobenzene-d5	7.422	82	716228	98.318	ng	0.00
42) 2,4,6-Tribromophenol	10.698	330	289426	156.322	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1194056	98.883	ng	0.00
79) Terphenyl-d14	12.986	244	969660	65.761	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122222\
Data File : BF131776.D
Acq On : 22 Dec 2022 14:37
Operator : CG\JU
Sample : N6102-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-7

Quant Time: Dec 23 01:53:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 01:24:08 2022
Response via : Initial Calibration




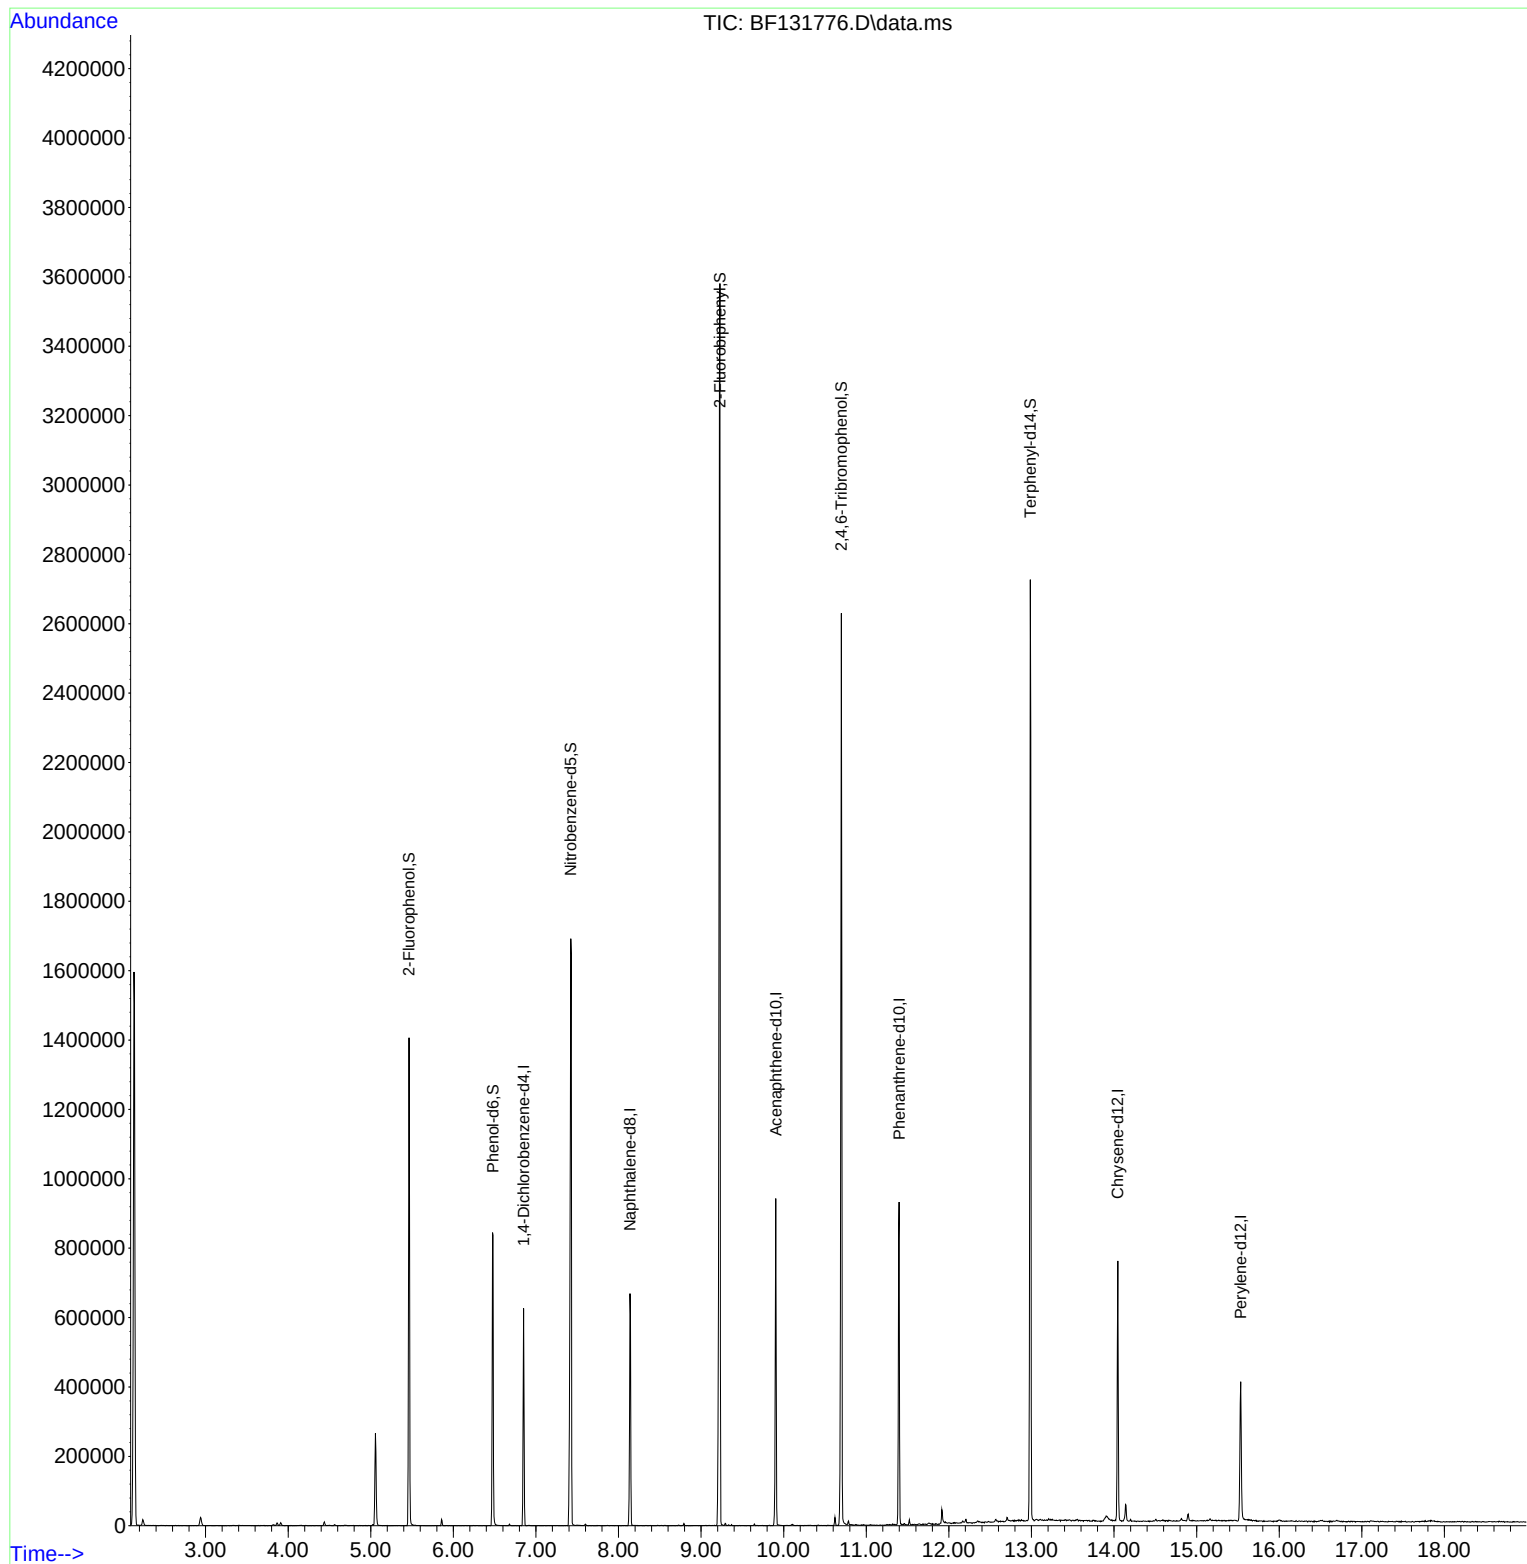




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.851 min Scan# 813
Delta R.T. -0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37




Instrument :
BNA_F
ClientSampleId :
MW-7


Tgt Ion:152 Resp: 80191
Ion Ratio Lower Upper
152 100
150 148.5 117.4 176.0
115 66.9 50.2 75.4

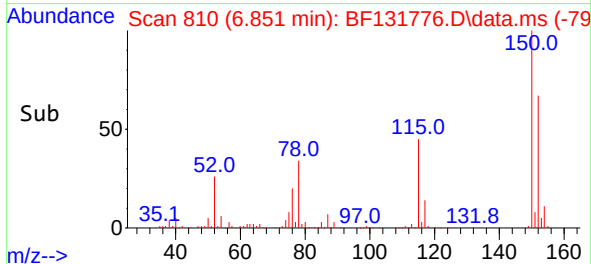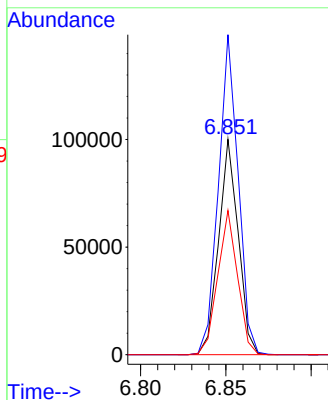

#5
2-Fluorophenol
Concen: 67.103 ng
RT: 5.463 min Scan# 574
Delta R.T. 0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37

Tgt Ion:112 Resp: 319560
Ion Ratio Lower Upper
112 100
64 67.3 49.5 74.3
63 37.2 28.2 42.2


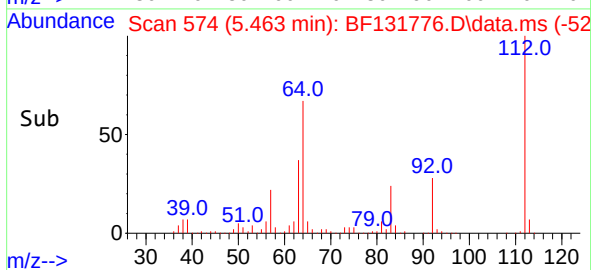
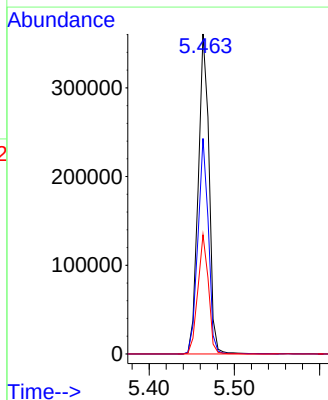
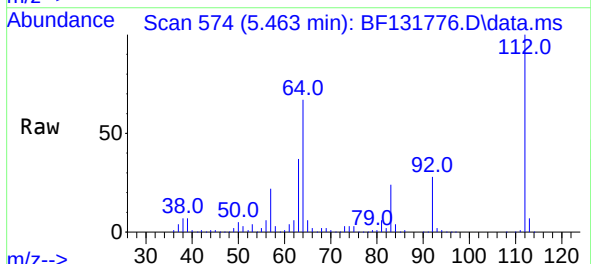




#7
Phenol-d6
Concen: 42.929 ng
RT: 6.481 min Scan# 74
Delta R.T. -0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37




Instrument :
BNA_F
ClientSampleId :
MW-7


Tgt Ion: 99 Resp: 275170
Ion Ratio Lower Upper
99 100
42 17.5 14.8 22.2
71 39.6 33.8 50.6

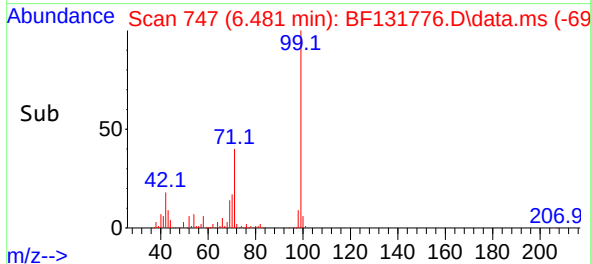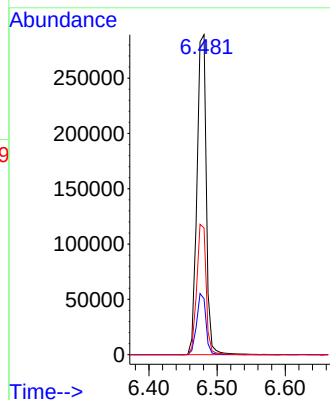

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.139 min Scan# 1029
Delta R.T. -0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37

Tgt Ion: 136 Resp: 295736
Ion Ratio Lower Upper
136 100
137 11.1 8.4 12.6
54 9.0 7.2 10.8
68 6.6 5.0 7.6


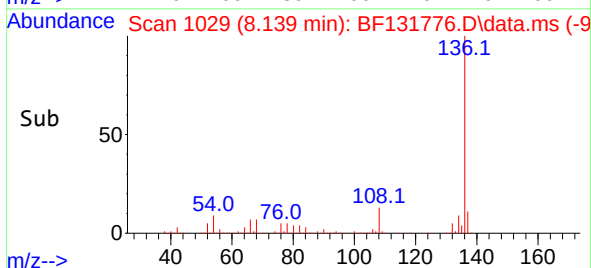
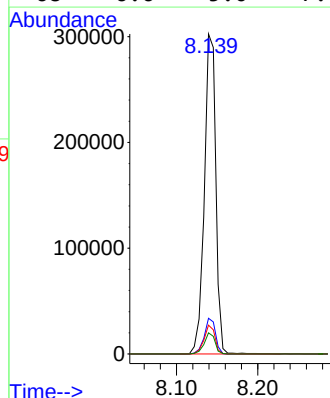
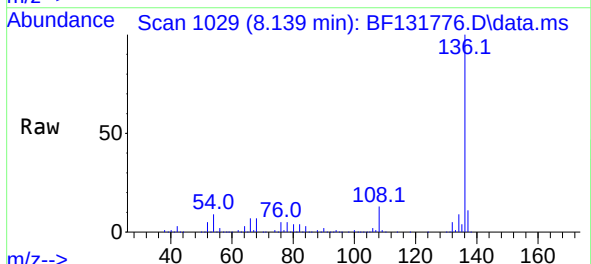


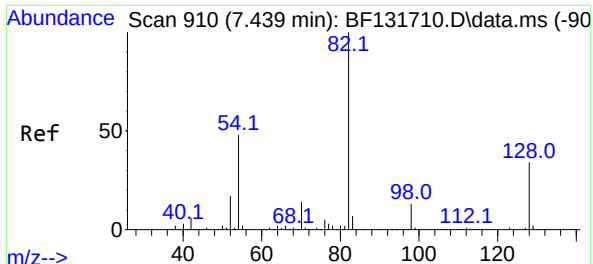

#23
Nitrobenzene-d5
Concen: 98.318 ng
RT: 7.422 min Scan# 907
Delta R.T. -0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37




Instrument :
BNA_F
ClientSampleId :
MW-7


Tgt Ion: 82 Resp: 716228
Ion Ratio Lower Upper
82 100
128 34.1 27.3 40.9
54 47.4 38.2 57.2

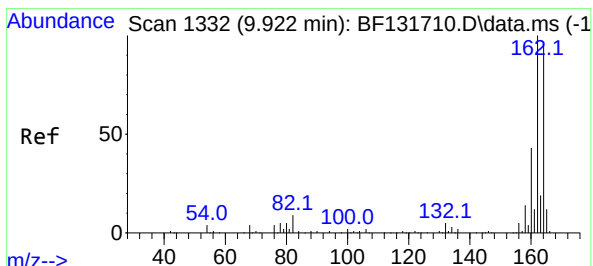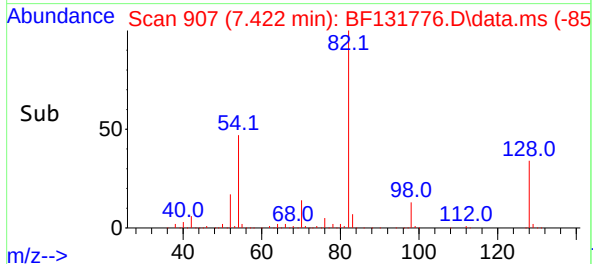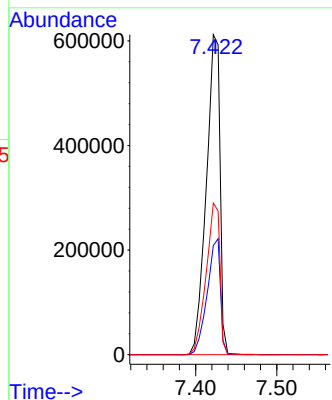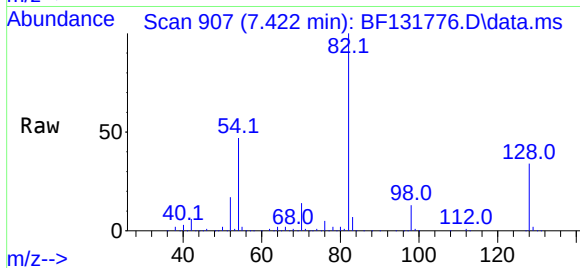

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.904 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37

Tgt Ion:164 Resp: 169156
Ion Ratio Lower Upper
164 100
162 102.8 83.7 125.5
160 44.7 36.2 54.4

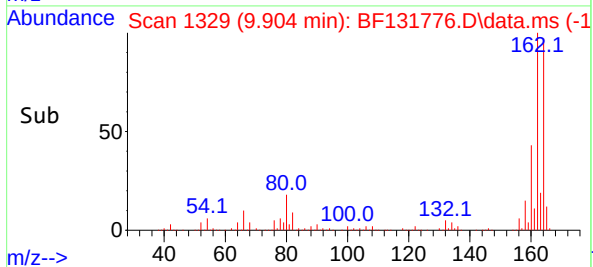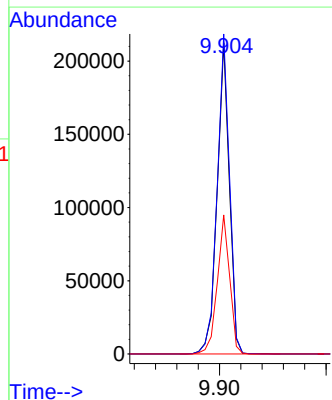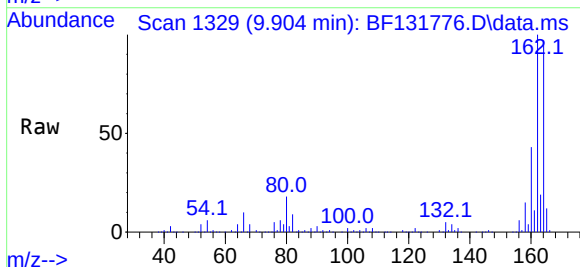



#42

2,4,6-Tribromophenol

Concen: 156.322 ng

RT: 10.698 min Scan# 1464

Delta R.T. -0.006 min

Lab File: BF131776.D

Acq: 22 Dec 2022 14:37

Instrument :

BNA_F

ClientSampleId :

MW-7





Tgt Ion:330 Resp: 289426

Ion Ratio Lower Upper

330 100

332 95.8 77.1 115.7

141 37.9 30.4 45.6

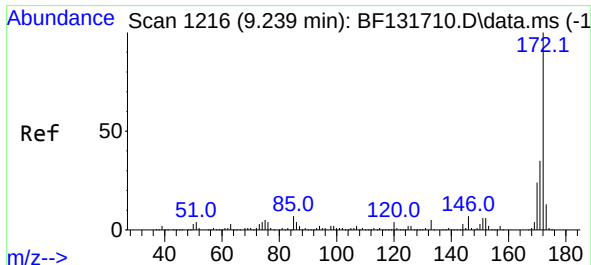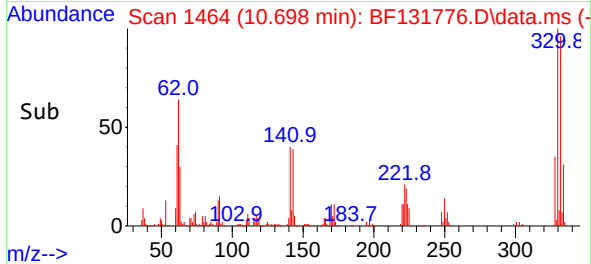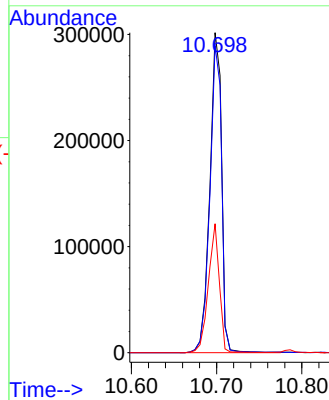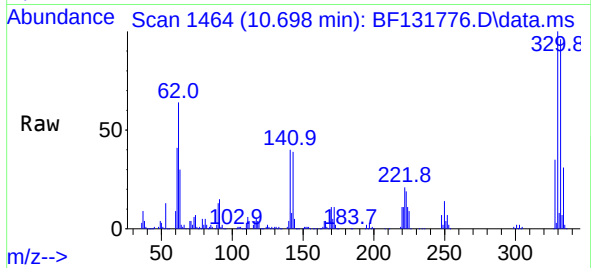

#45

2-Fluorobiphenyl

Concen: 98.883 ng

RT: 9.228 min Scan# 1214

Delta R.T. -0.000 min

Lab File: BF131776.D

Acq: 22 Dec 2022 14:37




Tgt Ion:172 Resp: 1194056


Ion Ratio Lower Upper

172 100

171 35.1 27.9 41.9

170 23.4 19.0 28.4


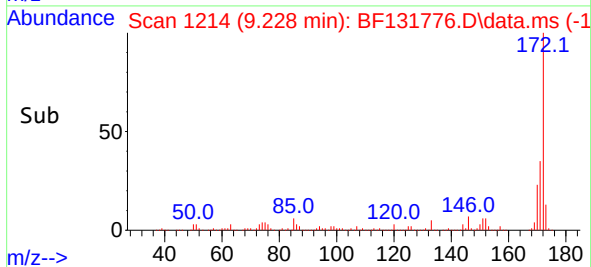
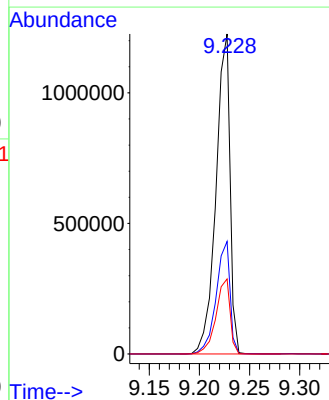
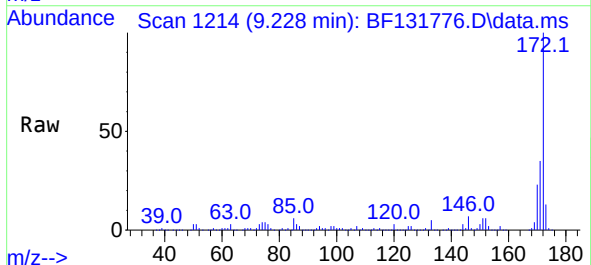




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37




Instrument :
BNA_F
ClientSampleId :
MW-7


Tgt Ion:188 Resp: 340542
Ion Ratio Lower Upper
188 100
94 6.9 5.9 8.9
80 8.4 7.0 10.6

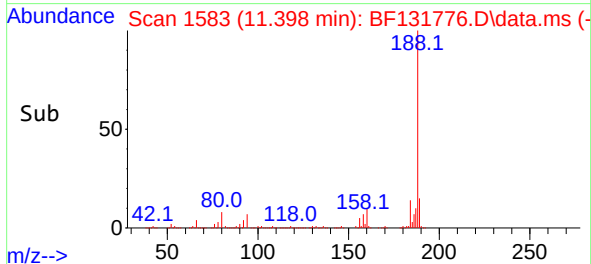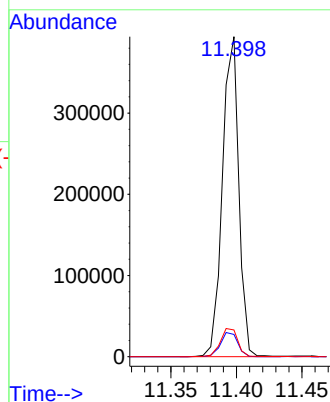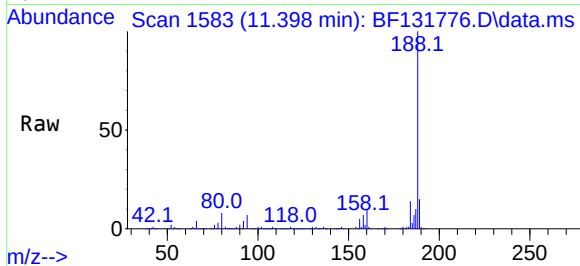

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2033
Delta R.T. -0.006 min
Lab File: BF131776.D
Acq: 22 Dec 2022 14:37

Tgt Ion:240 Resp: 229809
Ion Ratio Lower Upper
240 100
120 7.7 7.6 11.4
236 26.5 21.2 31.8


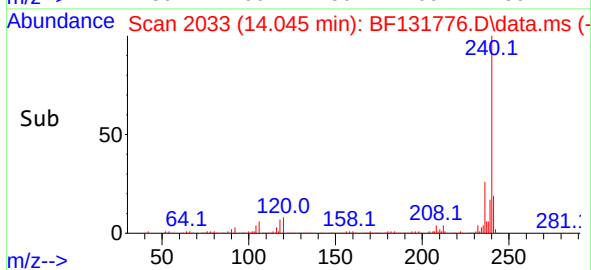
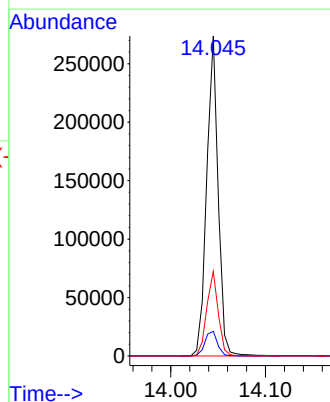
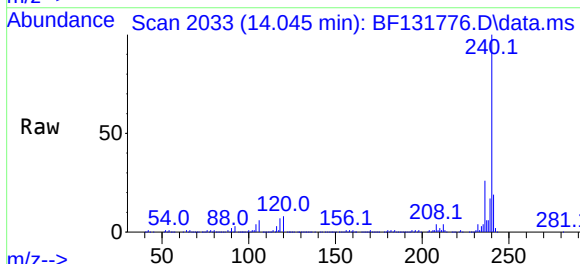




#79
 Terphenyl-d14
 Concen: 65.761 ng
 RT: 12.986 min Scan# 1856
 Delta R.T. -0.006 min
 Lab File: BF131776.D
 Acq: 22 Dec 2022 14:37

Instrument :
 BNA_F
 ClientSampleId :
 MW-7

Tgt Ion:244 Resp: 969660
 Ion Ratio Lower Upper
 244 100
 212 8.1 6.5 9.7
 122 9.6 7.7 11.5

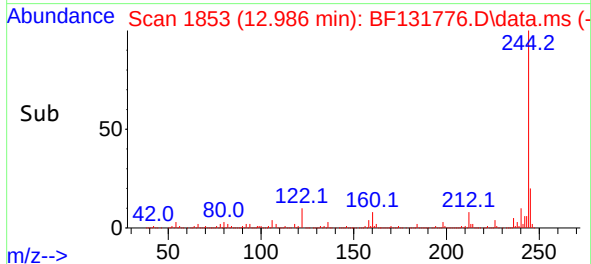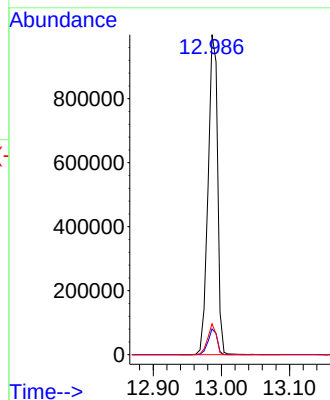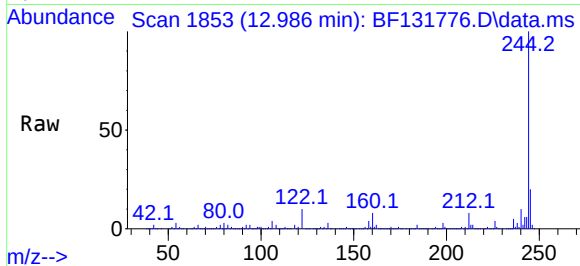

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.533 min Scan# 2286
 Delta R.T. -0.000 min
 Lab File: BF131776.D
 Acq: 22 Dec 2022 14:37

Tgt Ion:264 Resp: 183757
 Ion Ratio Lower Upper
 264 100
 260 22.7 18.6 28.0
 265 21.0 17.4 26.2

